

**Description and Results of the 2005 NIST/NOAA Interlaboratory
Comparison Exercise Program for Organic Contaminants in
Marine Mammal Tissues**

John R. Kucklick
Rebecca S. Pugh
Paul R. Becker
Michele M. Schantz
Dianne L. Poster
Stephen A. Wise
Teresa K. Rowles

Description and Results of the 2005 NIST/NOAA Interlaboratory Comparison Exercise Program for Organic Contaminants in Marine Mammal Tissues

**John R. Kucklick
Rebecca S. Pugh
Paul R. Becker**

*National Institute of Standards and Technology
Chemical Science and Technology Laboratory
Analytical Chemistry Division
Charleston Laboratory*

**Michele M. Schantz
Dianne L. Poster
Stephen A. Wise**

*National Institute of Standards and Technology
Chemical Science and Technology Laboratory
Analytical Chemistry Division*

Teresa K. Rowles

*National Oceanic and Atmospheric Administration
National Marine Fisheries Service*

March 2007



U.S. Department of Commerce
Carlos M. Gutierrez, Secretary

National Institute of Standards and Technology
William A. Jeffrey, Director

TABLE OF CONTENTS

LIST OF APPENDICES	iii
LIST OF TABLES	iv
ABSTRACT.....	vi
INTRODUCTION.....	1
MATERIALS USED IN THE 2005 EXERCISE	1
EVALUATION OF THE EXERCISE RESULTS.....	2
RESULTS AND DISCUSSION	7
CONCLUSIONS	8
LITERATURE CITED	9

LIST OF APPENDICES

- A. Tabular results of PCB congener, pesticide, PBDE congener, and lipid data reported by all laboratories****A1-A34**
- B. Graphical results of PCB congener and lipid data reported by all laboratories. The Z-scores for Homogenate VII represent 25% of the assigned value so that z = +1 is the assigned value plus 25 %, z = -1 is the assigned value minus 25 % and so forth. Error bars are \pm 1 standard deviation****B1-B28**
- C. Graphical results of pesticide and lipid data reported by all laboratories. The Z-scores for Homogenate VII represent 25% of the assigned value so that z = +1 is the assigned value plus 25 %, z = -1 is the assigned value minus 25 % and so forth. Error bars are \pm 1 standard deviation****C1-C18**
- D. Graphical results of PBDE congener data reported by all laboratories. The Z-scores for Homogenate VII represent 25% of the assigned value so that z = +1 is the assigned value plus 25 %, z = -1 is the assigned value minus 25 % and so forth. Error bars are \pm 1 standard deviation****D1-D5**
- E. Tabular summary of methods used for analysis by each laboratory.....****E1-E9**
- F. Additional analyte data and notes reported by individual laboratories.....****F1-F7**

LIST OF TABLES

Table 1: Laboratories Participating in the NIST/NOAA Interlaboratory Comparison Exercise Program for Organic Contaminants	3
Table 2a,b: Target and Optional Analytes for the NIST/NOAA Interlaboratory Comparison Exercise Program for Organic Contaminants in Marine Mammal Tissues.....	4-5
Table 3: Median organochlorine pesticide and lipid concentrations in Homogenate VII (Blainville's beaked whale; ng/g wet mass) reported by each laboratory. The values in bold were not used to derive the consensus value (see text for explanation)..	11
Table 4: Median PCB congener concentrations in Homogenate VII (Blainville's beaked whale; ng/g wet mass) reported by each laboratory. The values in bold were not used to derive the consensus value (see text for explanation)	12
Table 5: Median PBDE congener concentrations in Homogenate VII (Blainville's Beaked whale; ng/g wet mass) reported by each laboratory. The values in bold were not used to derive the consensus value (see text for explanation).	13
Table 6: Median organochlorine pesticide and lipid concentrations in SRM 1945 determined by each laboratory (ng/g wet mass and percent (mass fraction), respectively).....	14
Table 7: Median PCB congener concentrations in SRM 1945 determined by each laboratory (ng/g wet mass)...	15
Table 8: Median PBDE congener concentrations in SRM 1945 determined by each laboratory (ng/g wet mass).....	16
Table 9: Results from the analysis of Homogenate VII (Blainville's beaked whale) for fatty acids. Values are in percent (mass fraction). Fatty acids not requested for the exercise are given in Appendix F.....	17
Table 10: Results from the analysis of SRM 1945 for fatty acids. Values are in percent (mass fraction). Fatty acids not requested for the exercise are given in Appendix F. 2003 values are the median of results from three laboratories.....	18

DISCLAIMER

Certain commercial equipment or instruments are identified in this report to specify adequately the experimental procedures. Such identification does not imply recommendations or endorsement by the National Institute of Standards and Technology nor does it imply that the equipment or instruments are the best available for the purpose.

ABSTRACT

The National Institute of Standards and Technology (NIST), in support of the National Oceanic and Atmospheric Administration's Marine Mammal Health and Stranding Response Program (NOAA/MMHSRP), conducts annual interlaboratory comparison exercises for the determination of chlorinated pesticides, polychlorinated biphenyl congeners (PCBs), and trace elements in marine mammal tissues. These exercises provide one mechanism for laboratories to evaluate their measurement quality and comparability for these constituents in marine mammal tissues. In the 2005 exercise, 4 and 17 laboratories participated in determining the concentrations of selected fatty acids and PCBs and organochlorine pesticides, respectively, in a homogenized blubber control material "Marine Mammal Quality Assurance Exercise Homogenate VII" (Homogenate VII) and Standard Reference Material (SRM) 1945 Organics in Whale Blubber. This report includes the results reported by the participating laboratories, combined consensus data results, and summary statistics for each analyte in the samples. The numerical indices used to assess laboratory performance are also discussed.

INTRODUCTION

Laboratories measuring organic contaminants in the marine environment must assess the accuracy and precision of their measurements. Quality control of measurements made on marine environmental samples is vital to the accurate assessment of marine pollution and its effects on wildlife and human health. NIST aims to improve the quality of analytical measurements of organic contaminants in marine and environmental matrices by developing improved analytical methods, producing NIST Standard Reference Materials (SRMs) and other control materials, and conducting annual interlaboratory comparison exercises.

Through the NIST National Marine Analytical Quality Assurance Program and with support from the NOAA Marine Mammal Health and Stranding Response Program (MMHSRP), NIST conducts interlaboratory comparison activities to include analyses of marine mammal tissues. The 2005 NIST/NOAA Interlaboratory Comparison Exercise Program for Organic Contaminants in Marine Mammal Tissues was modeled after previous exercises (e.g., Schantz et al., 1996; Schantz et al., 2002; Kucklick et al., 2002, Kucklick et al., 2006). The current exercise was designed to help laboratories assess data comparability and quality relative to other groups providing measurements of organochlorine contaminants in marine mammal tissues and to link these important measurements to a national metrology laboratory. The results of the exercises presented in this report should be useful for both assessing current methodology and reducing the variability of contaminant data reported on marine mammals. Future exercises will allow for the assessment of analytical data quality over time. This report summarizes the 2005 organic contaminant exercise including methods used for analysis, data reported by the laboratories on the intercomparison materials, and numerical indices used to assess laboratory performance. A report describing the 2005 trace element results of this exercise is also available (Christopher et al. 2006).

MATERIALS USED IN THE 2005 EXERCISE

The 2005 NIST/NOAA Interlaboratory Comparison Exercise for Organochlorines in Marine Mammal Tissues (2005 MMQA) used two materials sent out to 24 laboratories. Twenty-one data sets from 18 laboratories were submitted for this exercise (Table 1). Seventeen data sets were submitted for organohalogen compounds and four for fatty acid compounds. Participants were asked to make three measurements each on two materials: SRM 1945 “Organics in Whale Blubber” and MMQA-VII (Homogenate VII), the “unknown.” The unknown material for the 2005 Organic Intercomparison Exercise was blubber from a male Blainville’s beaked whale (*Mesoplodon densirostris*) that stranded in North Carolina, USA. The tissues were homogenized and blended (Zeisler et al., 1983). At a NIST facility in Charleston, South Carolina, the blubber tissue was stored in a liquid nitrogen (LN₂) vapor phase freezer at -150 °C until prepared for this exercise. One bottle of this material containing approximately 10 g along with one bottle of SRM 1945 were sent either on dry ice or using a liquid nitrogen-cooled biological dry shipper via overnight express to each participating laboratory.

Exercise Requirements and Target Analytes

A suite of analytes was chosen for the exercise based on those tested in prior exercises (Schantz et al., 1996; Schantz et al., 2002; Kucklick et al., 2002; Kucklick et al., 2006) and several

additional analytes were included to broaden this list (Table 2a). In addition to the compounds listed in Table 2a, participants were requested to provide, if possible, values for polybrominated diphenyl ether (PBDE) congeners, coplanar polychlorinated biphenyl (PCB) congeners, total toxaphene and toxaphene congeners, chlorinated dioxins and furans and fatty acids (Table 2b). Laboratories were requested to make triplicate measurements of these compounds in each of the materials and to report their data using a data template provided by NIST. Results from the exercise were discussed during a workshop held in conjunction with the 2005 Society of Marine Mammology Biennial meeting in San Diego, California on December 13, 2005.

EVALUATION OF THE EXERCISE RESULTS

Determination of Laboratory Means and Consensus Values for Homogenate VII

Each laboratory reported the results of their analyses (Sample 1, Sample 2, and Sample 3) and the mean for each laboratory was calculated. The consensus value was calculated after comparing the results from an individual laboratory's analysis of SRM 1945 to the certified or reference value for the target organohalogens compounds given on the Certificate of Analysis for SRM 1945. If the value of a compound from a given laboratory for SRM 1945 was within 30 % of the reference value, the laboratory's result for the unknown sample was included in the calculation of the consensus value for the Homogenate VII. The median value for each compound was then calculated (Tables 3-5).

For the fatty acid portion of the exercise, the consensus value was not derived after screening the data as above. The 2005 exercise was only the second time participants were asked to measure fatty acids in SRM 1945 or an unknown; the first time was the 2003 exercise (Kucklick et al., 2006). The fatty acid consensus values for SRM 1945 from the 2003 exercise only consisted of results from three laboratories hence we did not feel it appropriate to use a consensus value based on such a small number of observations to screen data from the 2005 exercise.

Reported Results

Laboratories were assigned a random numerical identification code to shield the identity of the participants with the exception of NIST which was laboratories 1, 2, and 3. The same code was used for both materials. The results from the analysis of Homogenate VII and SRM 1945 are summarized in Tables 3 through 10. Appendix A shows the tabulated results from the individual laboratories for both materials and the results are shown graphically in Appendices B, C, and D. Appendix E gives the methods used for analysis by each laboratory and Appendix F shows data for additional analytes notes.

Table 1: Laboratories Participating in the 2005 NIST/NOAA Interlaboratory Comparison Exercise Program for Organic Contaminants.

Mississippi State Chemical Lab Mississippi State Mississippi State, Mississippi USA	Geochemical and Environmental Research Group Texas A&M University USA
California Animal Health and Food Safety Lab Toxicology UC Davis, School of Veterinary Medicine Davis, California USA	University of Pennsylvania Toxicology Laboratory Philadelphia, Pennsylvania USA
NOAA/National Ocean Service Hollings Marine Laboratory Charleston, South Carolina USA	Center for Marine Environmental studies, Ehime University Ehime, Japan Japan
NOAA/National Marine Fisheries Service Highlands, New Jersey USA	NOAA/National Marine Fisheries Service Northwest Fisheries Science Center Seattle, Washington USA (three data sets)
Laboratory of Environmental Toxicology The Norwegian School of Veterinary Science Oslo Norway	NIST Hollings Marine Laboratory Charleston, South Carolina USA
NOAA/National Ocean Service Center for Coastal Environmental Health and Biomolecular Research Charleston, South Carolina USA	NIST Gaithersburg, Maryland USA (two data sets)
Toxicological Center University of Antwerp (UA) Wilrijk Belgium	Mote Marine Laboratory Sarasota, Florida USA
Veterinary Medical Center Michigan State University East Lansing, Michigan USA	NOAA Auke Bay Laboratory Juneau, Alaska USA
Centre for Environment, Fisheries and Aquaculture Science CEFAS Burnham Laboratory Essex UK	Department of Biology University of Ottawa Ottawa, Ontario Canada

Table 2a: Target Analytes for the NIST/NOAA Interlaboratory Comparison Exercise Program for Organic Contaminants in Marine Mammal Tissues.

Pesticides	PCB Congeners	Substitution
2,4'-DDT	18	2,2',5
4,4'-DDT	28	2,4,4'
2,4'-DDE	31	2,4',5
4,4'-DDE	44	2,2',3,5'
2,4'-DDD	49	2,2',4,5'
4,4'-DDD	52	2,2',5,5'
HCB	66	2,3',4,4'
α -HCH	87	2,2',3,4,5'
γ -HCH	95	2,2',3,5',6l
β -HCH	99	2,2',4,4',5
heptachlor epoxide	101	2,2',4,5,5'
<i>cis</i> -chlordanane	105	2,3,3',4,4'
<i>trans</i> -chlordanane	118	2,3',4,4',5
oxychlordanane	128	2,2',3,3',4,4'
<i>cis</i> -nonachlor	132	2,2',3,3',4,6'
<i>trans</i> -nonachlor	138	2,2',3,4,4',5'
dieldrin	149	2,2',3,4',5',6
Mirex	151	2,2',3,5,5',6
	153	2,2',4,4',5,5'
	156	2,3,3',4,4',5
	170	2,2',3,3',4,4',5
	180	2,2',3,4,4',5,5'
	183	2,2',3,4,4',5',6
	187	2,2',3,4',5,5',6
	194	2,2',3,3',4,4',5,5'
	195	2,2',3,3',4,4',5,6
	201	2,2',3,3',4,5,5',6'
	206	2,2',3,3',4,4',5,5',6
	209	2,2',3,3',4,4',5,5',6,6'

Table 2b: Optional Analytes for the NIST/NOAA Interlaboratory Comparison Exercise Program for Organic Contaminants in Marine Mammal Tissues.

Compound	Substitution	Compound	Substitution
Polybrominated Diphenyl Ethers			Toxaphene
PBDE 47	2,2',4,4'	Total toxaphene	
PBDE 99	2,2',4,4',5	Toxaphene Congener 26	2-endo,3-exo,5-endo,6-exo,8,8,10,10-Octachlorobornane
PBDE 100	2,2',4,4,'6	Toxaphene Congener 50	2-endo,3-exo,5-endo,6-exo,8,8,9,10,10-Nonachlorobornane
PBDE 153	2,2',4,4',5,5'	Toxaphene Congener 62	2,2,5,5,8,9,9,10,10-Nonachlorobornane
PBDE 154	2,2',4,4',5,6'		
Fatty Acids			Coplanar PCBs
Lauric acid	C12:0	PCB 77	3,3',4,4'
Myristic acid	C14:0	PCB 126	3,3',4,4',5
Pentadecanoic acid	C15:0	PCB 169	3,3',4,4',5,5'
Palmitic acid	C16:0		
Margaric acid	C17:0	Chloro Dioxins and Furans	
Stearic acid	C18:0	Hexabromocyclodocecano	
Arachidic acid	C20:0	Isomers (α -, β -, and γ)	
Palmitoleic acid	C16:1(n-7)		
Vaccenic acid	C18:1(n-7)		
Oleic acid	C18:1(n-9)		
Elaidic acid	C18:1(n-9)		
	C20:1(n-7)		
Gondoic	C20:1(n-9)		
Gadoleic acid	C20:1(n-11)		
Erucic acid	C22:1(n-9)		
Cetoleic	C22:1(n-11)		
Nervonic acid	C24:1(n-9)		
Linoleic acid	C18:2(n-6)		
a-Linolenic acid	C18:3(n-3)		
g-linolenic acid	C18:3(n-6)		
Stearidonic acid	C18:4(n-3)		
Homo-gamma-linoleic acid	C20:2(n-6)		
Homo-alpha-linolenic acid	C20:3(n-3)		
Arachidonic acid	C20:4(n-6)		
EPA	C20:5(n-3)		
DPA	C22:2(n-6)		
DHA	C22:5(n-3)		
	C22:6(n-3)		

Assignment of z-and p-scores

Performance Scores: Different programs have different data quality needs. The acceptability of the results submitted by a laboratory will be decided by the individual program(s) for which the laboratory provides data. Typically, the program will use these exercise results in conjunction with the laboratory's performance in the analysis of certified reference materials and/or control materials, and of other quality assurance samples. These exercise results are shown in a number of ways in this report to aid in the evaluation of data quality.

IUPAC guidelines (IUPAC 1993) describe the use of "z-scores" and "p-scores" for assessment of accuracy and precision in interlaboratory comparison exercises, such as described in this report. These indices assess the difference between the result of the laboratory and the exercise assigned value, and can be used, with caution, to compare performance on different analytes and on different materials.

Accuracy Assessment (z-score):

$$z = \text{bias estimate} / \text{performance criterion}$$

or

$$z = (x - X)/\sigma$$

where x is the individual laboratory result, X is the "Exercise Assigned Value," and σ is the target value for the standard deviation. As described in the IUPAC guidelines, the choice of σ is dependent upon the data quality objective of a particular program. It can be fixed or determined by reference to validated methodology (*e.g.*, the calculated σ from the exercise data, see Tables 3 through 5). The fixed performance criterion is more useful in the comparison of a laboratory's performance on different materials, while the use of the actual variation may be more useful within a given exercise, for example, if the determination of a particular analyte is more problematic than usual.

The z-scores calculated using both approaches and applied to each laboratory's data are given in Appendix A. The same criterion was adopted for use in this exercise as was used in the former NIST/NOAA/NS&T program, where the target standard deviation was set to 25 % of the exercise assigned value. The z-scores for the Homogenate VII represent 25 % of the assigned value so that $z = +1$ is the assigned value plus 25 %, $z = -1$ is the assigned value minus 25 % and so forth. z-scores are also calculated based on the standard deviation of an analyte in the unknown material such that $z = +1$ is one "exercise standard deviation" higher than the assigned value and $z = -1$ is one "exercise standard deviation" lower than the assigned value and so forth. From a scientific point of view, IUPAC does not recommend the classification of z-scores, but does allow for such classification, *e.g.*,

$$|z| \leq 2 \quad \text{Satisfactory}$$

$$2 \leq |z| \leq 3 \quad \text{Questionable}$$

$$|z| \geq 3 \quad \text{Unsatisfactory}$$

The tables in Appendix A summarize the results and performance indices including the number of analytes that fall within each category for each laboratory.

Precision Assessment (p-score):

$$p = \sigma_{\text{lab}} / \sigma_{\text{target}} \approx \text{CV}_{\text{lab}} / \text{CV}_{\text{target}}$$

where σ_{lab} and σ_{target} are variance estimates for the individual laboratory and the target variance, respectively. The CV_{lab} is the coefficient of variance (or ratio of standard deviation to the mean), while the $\text{CV}_{\text{target}}$ is a target value chosen by the participants. During the workshop that accompanied this exercise, a target CV of 15 % was agreed upon, which is the same value used by other NIST run exercise programs (Schantz et al., 1996; Schantz et al., 2002; Kucklick et al., 2002; Kucklick et al., 2006). Note that the precision that p describes is that which occurs within a batch of analyses. Between-batch variance is likely larger and was not assessed in this exercise.

RESULTS AND DISCUSSION

Summarized results are shown in Tables 3 through 10 for the compounds listed in Tables 2a and 2b. Tabular results for individual laboratories are given in Appendix A, graphical results are given in Appendices B, C and D, and methods used by individual laboratories along with additional data and notes are given in Appendices E and F, respectively. Seventeen data sets were submitted for the organohalogen portion and four data sets were submitted for the fatty acid portion of the exercise. Fourteen data sets were submitted for pesticides, 12 for PCB congeners, and eight for the requested PBDE congeners. All except one laboratory had participated in the exercise before. For the 2003 exercise, 23 data sets were submitted for the organohalogen portion (PCB congeners and organochlorine pesticides) of the exercise and six data sets were submitted for the fatty acid portion (Kucklick et al., 2006).

The laboratories used a variety of methods to analyze the samples (Appendix E). For extraction, eight laboratories used pressurized fluid extraction, four used Soxhlet extraction, three used assisted extraction either with sonication or homogenization, two used liquid/liquid extraction, and one laboratory used column elution. Most laboratories (15) used internal standards, four laboratories used external standards, and one laboratory used a combination of internal and external standards. For detection, the most commonly used technique was gas chromatography-mass spectrometry (GC-MS; 10 laboratories), followed by GC-electron capture detection (GC-ECD; seven laboratories), GC-flame ionization detection (GC-FID; one lab for fatty acids), liquid chromatography diode array detection (one lab), and a combination of GC-MS and GC-ECD depending on compound class (one lab). All laboratories employing GC used capillary columns ranging in length from 25 m to 60 m. For organohalogen analysis, the most commonly used column was a 5 % phenyl methyl polysiloxane phase.

Based on the consensus values, Homogenate VII had considerably higher concentrations of total pesticides, PCBs, and PBDE congeners relative to SRM 1945 (Tables 3-8; Appendices B through D). The factor differences between Homogenate VII and SRM 1945 (i.e., Homogenate VII concentration/SRM 1945 concentration) were 9.7, 6.7, and 2.7 for the total organochlorine pesticides, total PCB congeners, and PBDE congeners, respectively, listed on Tables 3-8. The difference may be due to habitat, diet, or gender; SRM 1945 was collected from a mature female pilot whale while Homogenate VII was collected from a male Blainvilles's beaked whale. Concentrations of organohalogens are lower in female whales that have had calves relative to male or juvenile toothed whales (e.g., Tuerk et al. 2005).

The relative scatter of reported values seemed similar among compounds with some exceptions. The reported values for lipid (See Appendix C) were less than for the organohalogen compounds. PCB congener 201 showed somewhat of a bimodal distribution of values (Appendix A). For SRM 1945, the certified value for this compound is $16.8 \text{ ng/g} \pm 1.3 \text{ ng/g}$. However, four laboratories reported values averaging about 65 ng/g for this compound. It is likely that the laboratories were using the Zell and Ballschmiter nomenclature (Guitart et al., 1993) and are actually reporting the value for IUPAC congener 199 that has a reference value of $84.8 \text{ ng/g} \pm 2.2 \text{ ng/g}$ in SRM 1945. For the 2005 exercise, eight laboratories submitted data for the PBDEs which is three more laboratories than in 2003 (Kucklick et al., 2006). While several laboratories generally had good agreement with the certified values for the PBDE congener values in SRM 1945, a few labs had difficulty consistently obtaining values within 25 % of the certified value indicating that PBDE congener determination is still challenging for some laboratories (Appendix D).

This is the second exercise in which fatty acid analysis was requested. The values for individual fatty acids in SRM 1945 were on average within 25 % of the median of the 2003 results. For comparison, the median values for PCB congeners and organochlorine pesticides in SRM 1945 for the 2005 exercise were on average within 9 % of the certified values. The median fatty acid results from the 2003 and 2005 exercises will be compiled by NIST and listed on the Certificate of Analysis for SRM 1945.

CONCLUSIONS

Twenty-one laboratories submitted data for the two exercise materials on a wide variety of organic constituents including PCBs, pesticides, fatty acids, and PBDE congeners. The repeated participation of many laboratories in the exercise suggests that the exercise has been a useful tool for assessing their analytical performance. A new exercise will be conducted in 2007 using SRM 1945 and a new unknown material. The exercise coordinators plan to vary the type of control material used to include other species of interest such as a delphinid. NIST is somewhat constrained on the choice of the material as a fairly large quantity ($\approx 1 \text{ kg}$) is needed, and this amount of material is not available on a routine basis. SRM 1945 will continue to be the control material used in this exercise because it is the only marine mammal tissue available with certified and reference values for organochlorine compounds. During the meeting for participants held in conjunction with the Society of Marine Mammology biennial meeting, several laboratories indicated that a marine mammal plasma, serum, or whole blood should be

included as a matrix for the next exercise. NIST is attempting to obtain blood materials for this purpose. So far the attempts at obtaining a large enough pool of materials for the exercise have not been successful, however these attempts are continuing. It is likely that the blubber and blood exercises will not take place concurrently due to these difficulties.

LITERATURE CITED

- Christopher, S.J., Pugh, R.S., Ellisor, M.B., Mackey, E.A., Spatz, R.O., Porter, B.J., Bealer, K.J., Kucklick, J.R., Becker, P.R., and Rowles, T.K. National Marine Analytical Quality Assurance Program: Results and Description of the 2005 NIST/NOAA Interlaboratory Comparison Exercise for Trace Elements in marine Mammals. National Institute of Standards and Technology, NISTIR 7361.
- Guitart, R., Puig, P., and Gomez-Catalan, J. Requirement for a Standardized Nomenclature Criterion for PCBs: Computer-Assisted Assignment of Correct Congener Denomination and Numbering. *Chemosphere* 27:1451-1459 (1993).
- IUPAC. The International Harmonized Protocol for the Proficiency Testing of (Chemical) Analytical Laboratories; *Pure & Appl. Chem.* 65:123-2144 (1993).
- Kucklick, J.R., Christopher, S.J., Becker, P.R., Pugh, R.S., Porter, B.J., Schantz, M.M., Mackey, E.A., Wise, S.A., Rowles, T.K. Description and Results of the 2000 NIST/NOAA Interlaboratory Comparison Exercise Program for Organic Contaminants and Trace Elements in Marine Mammal Tissues. National Institute of Standards and Technology, NISTIR 6849 (2002).
- Kucklick J.R., Tuerk K.J.S., Vander Pol S.S, Schantz M.M., Wise SA. Polybrominated diphenyl ether congeners and toxaphene in selected marine standard reference materials. *Anal. Bioanal. Chem.* 378:1147-1151 (2004).
- Kucklick, J.R., Pugh, R.S., Becker, P.R., Schantz, M.M., Wise, S.A., and Rowles, T.K., Description and Results of the 2003 NIST/NOAA Interlaboratory Comparison Exercise Program for Organic Contaminants in Marine Mammal Tissues. National Institute of Standards and Technology, NISTIR 7269 (2006).
- Schantz, M.M., Wise, S.A., Segstro, M., Muir, D.C.G., and Becker, P.R. Interlaboratory Comparison Study for PCB Congeners and Chlorinated Pesticides in Beluga Whale Blubber. *Chemosphere* 33:1369-1390 (1996).
- Schantz, M.M., Kucklick, J.R., Parris, R.M., and Wise, S.A. NIST Intercomparison Exercise Program for Organic Contaminants in the Marine Environment. Description and Results of 2000 Organic Intercomparison Exercise. National Institute of Standards and Technology NISTIR 6837 (2002).

Tuerk K.J., Kucklick J.R., Becker P.R., Stapleton H.M., Baker J.E.. Persistent organic pollutants in two dolphin species with focus on toxaphene and polybrominated diphenyl ethers. *Environ. Sci. Technol.* 39:692-698 (2005).

Zeisler, R., Langland, J.K., and Harrison, J.K. Cryogenic Homogenization Procedure for Biological Tissues. *Anal. Chem.* 60: 2760-2765 (1983).

Table 3: Median organochlorine pesticide and lipid concentrations in Homogenate VII (Blainville's beaked whale; ng/g wet mass) reported by each laboratory. The values in bold were not used to derive the consensus value (see text for explanation).

Compound	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	Overall Median	1 SD	n	Consensus Median	1 SD	n
2,4'-DDT	572	1096	1473	433	333	295	523	1011	2250	1573	317	1826	792	670	12	428	304	6					
4,4'-DDT	2624	2427	2511	2320	2343	1432	3227	3170	2076	4023	4149	1112	1553	5021	2469	1108	14	2343	534	9			
2,4'-DDE	102.3	86.8	80.3	76.6	72.9	66.2	82.4				58.0		78.4	13.4	8	78.4	13	8					
4,4'-DDE	8694	6265	9927	7660	8630	6520	7143	10370	6969	5507	7166	2538	5703	8720	1055	7143	2515	15	7056	1733	12		
2,4'-DDD	111	73.5	84.9	96.6	125	110	116	198	670	75.0	47.7		110	175	11	97	43	9					
4,4'-DDD	1502	471	464	1323	1473	1076	2490	1248	1650	1361	760	983	1940	1286	1305	544	14	1286	412	10			
HCB	314	267	277	251	314	288	267	279	205	258	208		181	267	42	12	267	37	10				
alpha-HCH				4.59				6.25		3.66		3.50		4.12	1.3	4.0	4.12	1.3	4				
beta-HCH				3.27				13.8		5.79		7.03		6.41	4.5	4							
gamma-HCH								17.0	5.61	0.87		3.37		4.49	7.1	4	2.12	1.8	2				
Heptachlor Epoxide				48.8	49.6	59.2	63.8	51.1			16.3	69.7		89.4	55.1	21	8	49.2	19	4			
Cis-Chlordane	88.6	87.4	93.4	32.0	29.7	17.8	47.8			61.8	86.9	51.0	94.9	61.8	29	11	49.4	26	8				
Trans-Chlordane	7.79	19.9		7.62		7.14	16.8	41.2		1430		23.5		80.9	19.9	469	9	7.79	7.9	5			
Oxychlordane	275	350	321	265	240	252	232			275	155	237		258	53	10	258	53	10				
Cis-Nonachlor	218	232	242	256	198	248				672		227	209		232	149	9	232	17	7			
Trans-Nonachlor	1830	1888	1851	1410	1494	1360	1397			1737		1353	116		1452	515	10	1494	230	9			
Dieldrin	164	175	208	210	235	303	100	617			75.0	128	420		208	158	11	175	72	7			
Mirex	200	165	177	187	128	237.0		363		234		155		190	188	65.2	10	177	27	5			
Lipid	80.8	79.7	93.5	70.5	87.7	81.7	88.3	73.6	82.0	79.6	78.0	89.3	86	77.4	84.8	86.2	81.8	6.1	16	81.8	6	16	

Table 4: Median PCB congener concentrations in Homogenate VII (Blainville's beaked whale; ng/g wet mass) reported by each laboratory. The values in bold were not used to derive the consensus value (see text for explanation).

Congener(s)	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	Overall Median	1 SD	n	Consensus Median	1 SD	n	
18	8.39	4.75	3.46			8.40	30.8	32.0						4.2	6.84		7.62	12	8	6.57	13	4		
28	23.2	18.6	18.5	15.3			17.7	22.7	19.3					14.4	5.6		18.6	5.3	11	18.6	3.6	9		
31	1.76		2.69				3.0							0.0	0.80		2.69	6.5	5	1.76	0.7	3		
44	50.2	43.7	44.6	48.5		47.7	55.3	46.2	49.3					44.1	6.3		47.0	13.5	10	46.2	4.2	7		
49	88.7	89.1	86.0	92.7		96.7	98.8	85.0	101					69.6	25.8		88.9	22.1	10	88.7	10	7		
52	332	284	276	269		222	270	271	262					259.2	344		282	56	271	72	12	271	34	11
66/95*							380										380		1					
87		226	220	201				195									40	201	77	5	201	16	3	
99	558	460	490	426		477	465	466						483	324		352	234	465	92	11	465	68	11
101 (+90)	843	715	753	609	2953			653	645.0					579	465		1070	178	653	729	11	649	185	8
105	89.2	95.8	95.7	83.0	90.3	76.1	112	84.2	87.0					104.9	92		177	9.5	90.3	35	13	90.3	27	11
118	536	695	704	670	813		636	878	610					583	553		645	151	640	179	12	640	82	10
128	129	148	157	155	144		157		173					152	144		171	74	152	27	11	150	14	10
132							1907										127	29.5	127	1057	3		0	
138 (+163+164)	1902	1375	1388	1563	1377		1217	1273	1326					1507	1062		1670	343	1376	381	12	1377	230	11
149	833	743	761	741		859	697	605	636					653	793		720	185	731	175	12	741	80	11
151	330	251	277	261		262	277	210	242					294			254	0	261	32	10	261	32	10
153	2496	2534	1970	2207		1387		1831						1977	1703		1320	542	1900	600	10	1831	324	7
156	76.3	105	102	94.4	75.9	90.6	102	88.9	92.7					112	76.6		155		93.5	22	12	98.2	24	10
170 (+190)	307	286	301			291	281	306	334					305	257		248	72	291	70	11	296	25	10
180	908	830	909	834	890		800	827	915	890				1023	540		616	222	834	212	13	862	133	12
183	249	233	254	236		199	259	249	222					199	206		242	82	234	48	12	234	21	10
187	969	794	800	720		648	635	699	747					478	572		609	252	674	180	12	710	116	10
194	136	121	127	128		149	161	110	135					149	76.9		162	30	131	38	12	127	22	8
195	36.1	41.5	35.8	33.7		37.5	77.0	30.9									84	9.67	36.1	23	9	36.8	21	8
201	50.8	47.2	45.2	276		276	272	40.8									292	94	94.0	119	9	46.2	4.2	4
206	78.8	81.7	84.6	79.3		63.9	84.4	68.3						92.4			131	27.0	80.5	26	10	81.7	19	9
209	34.0	26.6	25.3	23.9		18.1	35.0	22.2						36.9			43	9.5	26.0	9.8	10	26.0	8.3	8
66	56.4	83.1	77.2	73.4		87.3		68.5	103					246			107	55.0	80.2	55	10	77.2	61	9
95	290	333	357	335		250									255		326		326	42	7	308	39	6

Table 5: Median PBDE congener concentrations in Homogenate VII (Blainville's Beaked whale; ng/g wet mass) reported by each laboratory. The values in bold were not used to derive the consensus value (see text for explanation).

Compound	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	Median	1 SD	n	Consensus Median	1 SD	n
PBDE 47	160			153		174		143			119	103	121		122			132	24	8	132	24	8
PBDE 99				26.3		43.5		26.6			21.7	19.2	22.2		76.0			26.3	20	7	22.2	3.2	5
PBDE 100	49.9			39.7		44.8		40.8			41.4	25.6	34.6		28.9			40.2	8.1	8	39.7	8.2	7
PBDE 153	17.1			15.4		26.1		16.1			13.1	12.6	12.6		35.3			15.8	8.1	8	14.2	2.0	6
PBDE 154	54.7			37.5		61.6		44.6			35.9	28.0	33.4		17.6			36.7	14	8	36.7	9.4	6

Table 6: Median organochlorine pesticide and lipid concentrations in SRM 1945 determined by each laboratory (ng/g wet mass and percent (mass fraction), respectively).

Compound	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	Median	1 SD	± 95% CI	n	Reference Value	Uncertainty	Comment
2,4'-DDT	97.7	94.9	134	57.5	85.4	85.3	101	130.7		220	178	71.0	266	99	64	36	12	90.9	13.5		certified value			
4,4'-DDT	255	220	239	169	229	196	362	251	216	440	372	383	180	370	245	89	46	14	233	8.02		certified value		
2,4'-DDE	16.8	12.5	11.1	14.2		17.4	14.3	14.2					17.3		14.2	2.3	1.6	8	14.2	1.39		certified value		
4,4'-DDE	519	470	851	516	477	482	509	687	452	407	510	355	412	454	85.7	477	162	82	15	497	19.5		certified value	
2,4'-DDD	22.0	17.9	21.2	18.5	24.7	53.2	25.1	21.7		93.3	18.0		19.7		21.7	23	14	11	19.55	1.18		certified value		
4,4'-DDD	120	126	86.7	117	114	152	199	96.0	153		102	78.2	106	160	167	119	35	18	14	119.9	4.87		certified value	
HCB	30.9	28.6	32.6	27.3	30.6	41.3	37.1	29.9	26.7			28.6	25.9	40.3	30.3	5.2	2.9	12	30.6	1.45		certified value		
alpha-HCH	21.1			16.1				17.6				13.9	7.30	13.0	20.3	16.1	4.7	3.5	7	16.9	1.41		certified value	
beta-HCH				5.02				11.2	10.4		2.0	5.03	6.33		5.68	3.5	2.8	6						
gamma-HCH	4.81			2.95				107	8.3		2.5		3.37	3.85	3.85	3.9	29	7	3.18	0.01		certified value		
Heptachlor Epoxide		10.7	10.3	10.0		23.9	17.9	15.4				9.57	16.3	14.0	14.0	4.7	3.1	9	10.7	0.09		certified value		
Cis-Chlordane	58.4	47.1	81.1	51.0		43.5	45.7	50.2			52.0	24.8	41.7	22.7	47.1	16	9.3	11	48.1	1.58		certified value		
Trans-Chlordane	12.4	11.8	5.65	11.2		11.1	20.2	27.0		145	15.1		12.7	70.7	12.7	42	25	11	11.8	0.54		certified value		
Oxychlordane	19.0	21.6	23.8	17.4		18.7	21.5	24.8			20.7	21.2	17.3		21.0	2.5	1.6	10	21.2	1.06		certified value		
Cis-Nonachlor	36.3	48.0	55.0	50.7		62.5		53.0			115		52.7	46.0	52.7	22	15	9	45.8	3.29		certified value		
Trans-Nonachlor	197	193	241	162		173	170	197			189		153	93.5	181	38	24	10	197.5	15.5		certified value		
Dieldrin	52.7	53.4	52.5	47.6		67.0	58.8	33.5	103			52.0	41.3	81.5	52.7	19	12	11	50.1	4.05		certified value		
Mirex	34.9	27.7	37.4	32.6		39.5	43.0		127		44.7		18.7		55.4	38.5	30	19	10	31.0	3.35		certified value	
Lipid	71.2	72.2	72.0	61.9	52.4	68.8	74.1	54.0	73.3	63	69.3	76.5	75.2	64.9	72.3	75.0	71.6	6.6	3.2	16	71.9	1.27		reference value

Table 7: Median PCB congener concentrations in SRM 1945 determined by each laboratory (ng/g wet mass).

Congener	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	Median	1 SD	± 95% CI	n	Reference Value	Uncertainty	Comment		
18	5.19	4.81	3.49			8.43	5.16	3.38						2.57	8.16		4.99	2.2	1.5	8	4.35	0.56	certified value			
28	13.5	12.5	9.91	10.5			13.8	14.8			10.5	12.4		11.5	5.68		11.9	2.6	1.6	10	13.1	1.07	certified value			
31	2.79	3.26	3.94	3.23							6.42			7.70	2.27		4.38	3.00	1.8	9	3.56	0.36	certified value			
44	11.3	11.2	11.3	12.8		16.9	13.0	13.5							10.9	4.05		11.3	3.4	2.2	9	12.1	0.51	certified value		
49	18.3	18.3	18.5	18.8		28.3	25.3	18.2	17.5						16.9	10.8		18.3	4.7	2.9	10	18.3	0.04	certified value		
52	43.0	42.2	39.8	38.1		36.3	47.5	38.3	31.0						38.4	43.9		34.4	18.5	7.5	12	40.7	1.30	certified value		
66/95*												64.0														
87																		12.6	22.8	6.2	5.4	5	20.6	2.55	certified value	
99	65.0	56.5	68.2	56.8		69.7	63.8	58.8							67.3	44.0		58.6	49.2	8.1	4.8	11	58.5	5.17	certified value	
101 (+90)	98.0	71.6	104.1	78.2	456										81.3	62.3		79.4	43.8	115	68	11	78.2	12.4	certified value	
105	26.7	26.5	30.8	28.1	31.6	31.0	37.7	24.7	32.3						31.5	29.5		25.3	10.8	6.3	3.4	13	28.6	1.16	certified value	
118	68.9	75.2	98.9	84.5	96.1			88.1	102.9	79.7					81.5	74.5		67.1	42.6	80.6	16	9.3	12	76.5	2.87	certified value
128	22.2	22.9	24.8	23.7	20.0			34.8	22.7	28.3					23.3	23.4		26.5	22.8	23.3	3.8	12	23.0	1.06	certified value	
132																		35.4	9.4	35.4	117	133	3	21.1	4.75	reference value
138 (+163+164)	182	143	166	189	144		165	137	156						170	133		173	84	161	28	16	12	146	12.9	certified value
149	103	95.0	99.2	84.1		98.3	95.5	70.1	80.7						69.6	95.7		74.1	39.6	89.6	18	10	12	89.0	6.94	certified value
151	32.3	26.8	32.5	27.8		31.7	32.2	21.1	26.7						32.5			27.8	9.5	5.6	11	28.6	1.33	certified value		
153	300	334	249	279	0.0	201		215							245	211		181	109	230	64	40	10	228	9.75	certified value
156	10.2	11.0	14.0	12.3	8.02	15.8	14.6	10.9	16.0						13.4	10.2		12.6		12.4	2.5	1.4	12	11.4	0.95	certified value
170 (+190)	43.9	43.4	46.9				47.1	40.3	44.1	49.0					44.3	39.1		33.0	25.6	43.9	6.9	4.1	11	42.6	2.18	certified value
180	148	133	169	143	141	141	165	157	160						153	100		107	73.1	143	28	15	13	138.3	9.70	certified value
183	39.3	35.1	44.7	39.9		37.4	49	42.3	38.7						37.7	36.6		30.5	21.3	38.2	7.0	4.0	12	38.04	1.83	certified value
187	150	113	146	116		117	130	116	124						83.9	103		97.0	64.0	116	24	14	12	121.5	11.1	certified value
194	64.6	47.2	60.3	55.7		78.8	77.9	50.3	61.0						60.3	37.7		32.0	29.9	58.0	16	9.0	12	53.5	5.18	certified value
195	14.0	12.6	11.5	10.3		15.4	11.6	12.5									15.3	5.23	12.5	3.1	2.0	9	14.3	2.17	certified value	
201	16.7	16.2	15.8	80.2		24.9	87.5	13.1									53.7	43.0	24.9	29	18.9	9	16.8	1.30	certified value	
206	50.5	43.8	54.3	48.5		39.8	51.8	44.0							52.9			35.9	25.5	46.3	9.0	5.6	10	44.9	4.23	certified value
209	18.7	18.9	20.5	18.1		13.3	25.5	19.0									19.8	14.6	10.4	18.8	4.2	2.6	10	17.2	1.86	certified value
66	22.3	22.9	26.7	22.2		30.5	21.8	26.7									25.4	22.2	18.2	22.6	3.5	2.1	10	22.4	0.51	certified value
95	33.3	33.5	47.9	39.6		39.3		35.0									33.0	39.8		37.1	5.1	3.5	8	33.9	0.51	certified value

Table 8: Median PBDE congener concentrations in SRM 1945 determined by each laboratory (ng/g wet mass).

Congener	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	Median	1 SD	± 95% CI	n	Reference Value	Uncertainty	Comment
PBDE 47	39.7			37.0		51.5	40.9			35.5	37.8	36.4		32.3			37.4	5.7	4.0	8	39.6	0.18	certified value	
PBDE 99				15.4		29.4	17.6			16.5	16.5	16.4		46.9			16.5	12	8.7	7	18.9	2.32	certified value	
PBDE 100	12.0			8.44		16.4	9.51			10.3	9.24	9.10		9.39			9.45	2.6	1.8	8	10.3	1.13	certified value	
PBDE 153	8.01			7.46		17.3	7.16			8.33	8.38	7.50		12.6			8.17	3.6	2.5	8	8.34	0.55	certified value	
PBDE 154	10.9			11.3		30.8	12.3			12.4	13.0	10.9		8.26			11.8	7.0	4.9	8	13.3	1.73	certified value	

Table 9: Results from the analysis of Homogenate VII (Blainville's beaked whale) for fatty acids. Values are in percent (mass fraction). Fatty acids not requested for the exercise are given in Appendix F.

Compound (Synonyms)			Laboratory				Median	1 SD
			18	19	20	21		
Lauric acid	Dodecanoic acid	C12:0	0.082	0.080	0.059	0.092	0.078	0.01
Myristic acid	Tetradecanoic acid	C14:0	0.72	1.51	1.19	1.72	1.28	0.44
Pentadecanoic acid	Pentadecanoic acid	C15:0	0.075	0.073	0.052	0.084	0.071	0.01
Palmitic acid	Hexadecanoic acid	C16:0	0.98	2.44	1.78	2.64	1.96	0.75
Margaric acid	Heptadecanoic acid	C17:0	0.058	0.050	0.043	0.071	0.055	0.01
Stearic acid	Octadecanoic acid	C18:0	0.65	0.71	0.48	0.89	0.68	0.17
Arachidic acid	Eicosanoic acid	C20:0	0.082	0.12	0.054	0.16	0.10	0.05
Palmitoleic acid	(Z)-9-Hexadecanoic acid	C16:1(n-7)	3.04	3.09	2.34	3.54	3.00	0.49
Vaccenic acid	(Z)-11-Octadecenoic acid	C18:1(n-7)	1.31	1.25	0.99	1.49	1.26	0.21
Oleic acid	(Z)-9-Octadecanoic acid	C18:1(n-9)	18.3	13.4	8.00	15.2	13.7	4.3
Elaidic acid	(E)-9-Octadecenoic acid	C18:1(n-9)						
	(Z)-13-eicosenoic acid	C20:1(n-7)		0.26	0.25	0.35	0.29	0.06
Gondoic	(Z)-11-eicosenoic acid	C20:1(n-9)	6.09	7.09	4.62	8.17	6.49	1.51
Gadoleic acid	(Z)-9-Eicosenoic acid	C:20:1(n-11)	5.91	5.04	3.32	5.69	4.99	1.17
Erucic acid	(Z)-13-Docosenoic acid	C22:1(n-9)	0.73	0.73	0.42	1.11	0.75	0.28
Cetoleic	(Z)-11-docosenoic acid	C22:1(n-11)	5.94	4.64	3.06	5.41	4.76	1.26
Nervonic acid	(Z)-15-Tetracosenoic acid	C24:1(n-9)	0.19	0.15	0.08	0.20	0.16	0.05
Linoleic acid	(Z,Z)-9,12-Octadecadienoic acid	C18:2(n-6)	0.47	0.41	0.03	0.54	0.36	0.23
a-Linolenic acid	(Z,Z,Z)-9,12,15-Octadecatrienoic acid	C18:3(n-3)	0.54	0.083		0.17	0.26	0.24
g-linolenic acid	(Z,Z,Z)-6,9,12-Octadecatetraenoic acid	C18:3(n-6)	0.011	0.010		0.022	0.014	0.01
Stearidonic acid	(Z,Z,Z,Z)-6,9,12,15-Octadecatetraenoic acid	C18:4(n-3)	0.079	0.143		0.090	0.10	0.03
Homo-gamma-linoleic acid	(Z,Z)-11,14-Eicosadienoic acid	C20:2(n-6)	0.15	0.067		0.17	0.13	0.06
Homo-alpha-linolenic acid	(Z,Z,Z)-11,14,17-Eicosatrienoic acid	C20:3(n-3)		0.030		0.066	0.048	0.03
Arachidonic acid	(Z,Z,Z,Z)-5,8,11,14-Eicosatetraenoic acid	C20:4(n-6)	0.13	0.12	0.04	0.18	0.12	0.06
EPA	(Z,Z,Z,Z,Z)-5,8,11,14,17-Eicosapentaenoic acid	C20:5(n-3)	0.38	0.31	0.11	0.51	0.33	0.17
	(Z,Z)-13,16-Docosadienoic acid	C22:2(n-6)	0.031			0.033	0.032	
DPA	(Z,Z,Z,Z,Z)-7,10,13,16,19-Docosapentaenoic acid	C22:5(n-3)	0.29	0.20	0.08	0.47	0.26	0.17
DHA	(Z,Z,Z,Z,Z,Z)-4,7,10,13,16,19-Docosahexaenoic Acid	C22:6(n-3)	0.86	0.57	0.10	0.85	0.59	0.36

Table 10: Results from the analysis of SRM 1945 for fatty acids. Values are in percent (mass fraction). Fatty acids not requested for the exercise are given in Appendix F. 2003 values are the median of results from the laboratories.

Compound (Synonyms)			Laboratory				2003 Values			
			18	19	20	21	Median	1 SD	Median	1 SD
Lauric acid	Dodecanoic acid	C12:0	0.19	0.15	0.13	0.19	0.16	0.03	0.20	0.09
Myristic acid	Tetradecanoic acid	C14:0	0.87	3.13	2.71	3.63	2.59	1.20	3.44	1.2
Pentadecanoic acid	Pentadecanoic acid	C15:0	0.25	0.30	0.23	0.36	0.28	0.06	0.36	0.08
Palmitic acid	Hexadecanoic acid	C16:0	1.22	7.51	5.96	7.41	5.52	2.96	7.13	3.5
Margaric acid	Heptadecanoic acid	C17:0	0.16	0.22	0.16	0.25	0.20	0.05	0.25	0.09
Stearic acid	Octadecanoic acid	C18:0	0.83	1.25	1.11	1.43	1.16	0.25	1.36	0.38
Arachidic acid	Eicosanoic acid	C20:0	0.069	0.10	0.075	0.14	0.10	0.03	0.11	0.02
Palmitoleic acid	(Z)-9-Hexadecanoic acid	C16:1(n-7)	5.08	5.75	4.50	6.46	5.45	0.85	6.47	1.8
Vaccenic acid	(Z)-11-Octadecenoic acid	C18:1(n-7)	1.59	1.80	1.61	2.00	1.75	0.19	2.04	0.7
Oleic acid	(Z)-9-Octadecanoic acid	C18:1(n-9)	17.8	13.9	10.9	15.2	14.4	2.83	16.7	2.5
Elaidic acid	(E)-9-Octadecenoic acid	C18:1(n-9)							0.21	0.08
	(Z)-13-eicosenoic acid	C20:1(n-7)		0.24	0.18	0.27	0.23	0.04		
Gondoic	(Z)-11-eicosenoic acid	C20:1(n-9)	4.24	4.67	3.54	5.27	4.43	0.73	5.04	1.9
Gadoleic acid	(Z)-9-Eicosenoic acid	C20:1(n-11)	3.05	2.94	2.48	3.25	2.93	0.33	1.41	1.6
Erucic acid	(Z)-13-Docosenoic acid	C22:1(n-9)	0.47	0.51	0.44	0.80	0.56	0.17	0.70	0.20
Cetoleic	(Z)-11-docosenoic acid	C22:1(n-11)	5.14	4.61	3.32	5.17	4.56	0.86	4.12	
Nervonic acid	(Z)-15-Tetracosenoic acid	C24:1(n-9)	0.29	0.22	0.13	0.30	0.24	0.08	0.30	
Linoleic acid	(Z,Z)-9,12-Octadecadienoic acid	C18:2(n-6)	0.75	0.75	0.11	0.91	0.63	0.36	0.91	0.30
a-Linolenic acid	(Z,Z,Z)-9,12,15-Octadecatrienoic acid	C18:3(n-3)	0.35	0.32		0.40	0.36	0.04	0.62	0.21
g-linolenic acid	(Z,Z,Z)-6,9,12-Octadecatetraenoic acid	C18:3(n-6)	0.018	0.020		0.026	0.021	0.004	0.02	0.01
Stearidonic acid	(Z,Z,Z,Z)-6,9,12,15-Octadecatetraenoic acid	C18:4(n-3)	0.21	0.23		0.20	0.21	0.02	0.18	
Homo-gamma-linoleic acid	(Z,Z)-11,14-Eicosadienoic acid	C20:2(n-6)	0.22	0.17		0.030	0.14	0.10	0.24	0.09
Homo-alpha-linolenic acid	(Z,Z,Z)-11,14,17-Eicosatrienoic acid	C20:3(n-3)	0.14	0.13		0.19	0.16	0.03	0.18	
Arachidonic acid	(Z,Z,Z,Z)-5,8,11,14-Eicosatetraenoic acid	C20:4(n-6)	0.23	0.22	0.08	0.31	0.21	0.10	0.30	
EPA	(Z,Z,Z,Z)-5,8,11,14,17-Eicosapentaenoic acid	C20:5(n-3)	1.09	1.12	0.54	1.27	1.00	0.32	1.44	0.32
	(Z,Z)-13,16-Docosadienoic acid	C22:2(n-6)	0.02			0.04	0.029	0.01	0.018	0.01
DPA	(Z,Z,Z,Z)-7,10,13,16,19-Docosapentaenoic acid	C22:5(n-3)	1.00	0.88	0.48	0.94	0.83	0.23	1.05	0.3
DHA	(Z,Z,Z,Z,Z)-4,7,10,13,16,19-Docosahexaenoic Acid	C22:6(n-3)	3.34	3.70	0.88	4.33	3.06	1.51	4.42	1.5

Appendix A

Tabular results of PCB congener, pesticide, PBDE congener, and lipid data reported by all laboratories.

PESTICIDE, PBDE, AND LIPID ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)										Material Reference Values (ng/g wet mass)				Performance Scores ^a		
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		z-score (25%)	Homog VII z-score (s)	p-score (15%)
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	Uncert			
2,4'-DDT	573	569	576	92.9	100	100	572	0.6	97.7	4.2	428	243	90.9	13.5	1.4	0.5	0.0
4,4'-DDT	2577	2621	2673	255	254	256	2624	1.8	255	0.4	2343	349	233	8.02	0.5	0.5	0.1
2,4'-DDE	105	105	97.1	17.4	16.9	16.1	102	4.5	16.8	4.0	78.4	9.3	14.2	1.39	1.2	1.8	0.3
4,4'-DDE	8882	8621	8578	517	509	531	8694	1.9	519	2.1	7056	981	497	19.5	0.9	0.9	0.1
2,4'-DDD	118	109	107	22.8	21.2	21.8	111	5.3	22.0	3.5	96.6	28	19.5	1.18	0.6	0.3	0.4
4,4'-DDD	1486	1499	1521	120	120	121	1502	1.2	120	0.2	1286	255	120	4.87	0.7	0.5	0.1
HCB	321	314	308	31.0	29.1	32.7	314	2.0	30.9	5.9	267	23	30.6	1.45	0.7	1.3	0.1
α-HCH	<2	<2	<2	20.1	18.9	24.2	<2		21.1	13.3	4.12	1.2	16.9	1.41			
β-HCH	<2	<2	<2	<2	<2	<2											
γ-HCH	<2	<2	<2	4.85	4.39	5.18	<2		4.81	8.2	2.12	2.5	3.18	0.01			
Heptachlor Epoxide	<10	<10	<10	<10	<10	<10	<10				49.2	18	10.7	0.09			
Cis-Chlordane	83.2	92.6	89.9	59.9	59.8	55.6	89	5.4	58.4	4.2	49.4	18	48.1	1.58	3.2	1.5	0.4
Trans-Chlordane	7.76	7.07	8.55	11.8	12.5	13.0	7.79	9.5	12.4	4.6	7.79	6.9	11.8	0.54	0.0	0.0	0.6
Oxychlordane	261	300	264	18.9	19.7	18.5	275	7.9	19.0	3.1	258	33	21.2	1.06	0.3	0.3	0.5
Cis-Nonachlor	208	217	229	33.7	36.7	38.6	218	4.9	36.3	6.8	232	12	45.8	3.29	-0.2	-0.8	0.3
Trans-Nonachlor	1751	1768	1972	193	192	205	1830	6.7	197	3.9	1494	150	198	15.5	0.9	1.5	0.4
Dieldrin	171	150	171	49.1	54.9	54.0	164	7.4	52.7	5.9	175	53	50.1	4.05	-0.3	-0.2	0.5
Mirex	197	206	196	31.8	35.4	37.4	200	2.9	34.9	8.1	177	24	31.0	3.35	0.5	0.8	0.2
PBDE 47	152	160	167	38.3	40.7	40.0	160	4.7	39.7	3.1	132	17	39.6	0.18	0.8	1.1	0.3
PBDE 99	inf*	inf	inf	inf	inf	inf					22.2	2.8	18.9	2.32			
PBDE 100	45.8	49.1	54.7	11.7	12.7	11.6	49.9	9.0	12.0	5.1	39.7	6.1	10.3	1.13	1.0	1.2	0.6
PBDE 153	16.7	17.5	17.2	7.93	8.13	7.96	17.1	2.3	8.01	1.4	14.2	1.6	8.34	0.55	0.8	1.4	0.2
PBDE 154	54.0	52.9	57.2	10.4	10.4	12.0	54.7	4.1	10.9	8.7	36.7	7.5	13.3	1.73	2.0	1.9	0.3
Lipid (mass fraction (%))	82.1	80.3	80.1	71.8	70.8	71.1	80.8	1.40	71.2	0.74	80.5	3.3	71.9	1.27	0.0	0.0	0.1

^aCertified values are in bold^bSee text for explanation

Category	Number by Category		
	z (25%)	z (s)	p (15%)
	≤ 2	2 to 3	≥ 3
	18	19	19
	0	0	0
	1	0	0
	z (25%)	z (s)	p (15%)

PCB CONGENER ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)										Material Reference Values (ng/g wet mass)				Performance Scores ^a		
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		z-score (25%)	Homog VII z-score (s)	p-score (15%)
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	Uncert			
18	8.19	8.11	8.88	5.23	5.19	5.15	8.39	5	5.2	0.9	6.57	12.6	4.35	0.56	1.1	0.1	0.3
28	22.9	22.4	24.4	13.9	13.2	13.3	23.2	4.5	13.5	2.6	18.6	2.4	13.06	1.07	1.0	1.3	0.3
31	<2	<2	<2	2.9	2.7	2.7	<2		2.8	3.5	1.76	0.7	3.56	0.36			
44	46.9	52.2	51.4	11.5	11.1	11.3	50.2	5.7	11.3	1.7	46.2	3.1	12.1	0.51	0.3	0.9	0.4
49	84.7	91.0	90.4	18.3	18.4	18.1	88.7	3.9	18.3	0.6	88.7	7.0	18.3	0.04	0.0	0.0	0.3
52	333	328	335	41.7	43.3	43.9	332	1.1	43.0	2.6	271	20	40.7	1.30	0.9	1.8	0.1
66/95*	below	below	below	below	below	below	below		below								
87	inf*	inf	inf	inf	inf	inf	inf		inf		201	18	20.6	2.55			
99	592	561	520	65.4	63.0	66.5	558	6.5	65.0	2.7	465	40	58.5	5.17	0.8	1.4	0.4
101 (+90)	870	852	806	97.5	97.0	99.4	843	3.9	98.0	1.3	649	129	78.2	12.4	1.2	1.0	0.3
105	91.1	86.3	90.0	27.0	25.8	27.4	89.2	2.8	26.7	3.1	90	16	28.6	1.16	0.0	0.0	0.2
118	541	531	536	68.5	67.7	70.6	536	0.9	68.9	2.2	640	51	76.5	2.87	-0.7	-1.3	0.1
128	127	126	134	22.4	22.2	22.1	129	3.1	22.2	0.7	150	8.6	23.0	1.06	-0.6	-1.5	0.2
132	w/153	w/153	w/153	w/153	w/153	w/153	w/153		w/153								
138 (+163+164)	1867	1876	1963	174	181	192	1902	2.8	182	5.1	1377	136	146	12.9	1.5	2.3	0.2
149	849	831	818	103.5	101.8	103.6	833	1.9	103	1.0	741	47	89.0	6.94	0.5	1.1	0.1
151	330	333	327	32.3	32.3	32.2	330	0.9	32.3	0.2	261	20	28.6	1.33	1.0	2.1	0.1
153	2489	2476	2522	301	297	302	2496	1.0	300	0.9	1831	240	228	9.75	1.5	2.1	0.1
156	77.2	72.1	79.5	9.9	10.1	10.5	76.3	5.0	10.2	3.0	98.2	15	11.4	0.95	-0.9	-0.9	0.3
170 (+190)	296	314	312	45.7	41.5	44.6	307	3.2	43.9	5.0	296	16	42.6	2.18	0.2	0.5	0.2
180	880	919	924	150	145	148	908	2.7	148	1.7	862	75	138	9.70	0.2	0.3	0.2
183	235	264	248	39.7	38.8	39.5	249	5.9	39.3	1.2	234	13	38.0	1.83	0.3	0.7	0.4
187	932	1006	970	148	147	155	969	3.8	150	2.8	710	72	121	11.1	1.5	2.2	0.3
194	133	142	132	63.0	65.2	65.6	136	4.1	64.6	2.2	127	15	53.5	5.18	0.3	0.4	0.3
195	38.0	35.0	35.2	13.8	13.6	14.5	36.1	4.6	14.0	3.3	37	14	14.3	2.17	-0.1	0.0	0.3
201	50.0	55.5	46.8	16.7	16.2	17.4	50.8	8.6	16.7	3.8	46.2	4.1	16.8	1.30	0.4	1.1	0.6
206	82.5	75.0	78.9	49.8	51.2	50.5	78.8	4.8	50.5	1.4	81.7	13	44.9	4.23	-0.1	-0.2	0.3
209	32.6	32.0	37.5	17.8	19.8	18.5	34.0	8.8	18.7	5.3	26.0	5.7	17.2	1.86	1.2	1.0	0.6
66	54.0	55.8	59.4	22.0	22.4	22.5	56.4	4.9	22.3	1.2	77.2	40	22.4	0.51	-1.1	-0.3	0.3
95	307	293	270	33.6	32.9	33.4	290	6.5	33.3	1.1	308	31	33.9	0.51	-0.2	-0.5	0.4

^aCertified values are in bold ^bSee text for explanation

*interference

Category	Number by Category		
	z (25%)	z (s)	p (15%)
≤ 2	26	22	26
2 to 3	0	4	0
≥ 3	0	0	0

PESTICIDE, PBDE, AND LIPID ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)										Material Reference Values (ng/g wet mass)				Performance Scores ^a		
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		Homog VII	z-score (25%)	
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	Uncert	z-score (s)	p-score (15%)	
2,4'-DDT	1079	1066	1144	96.7	93.6	94.5	1096	3.8	94.9	1.7	428	243	90.9	13.5	6.3	2.2	0.3
4,4'-DDT	2390	2450	2440	221	207	231	2427	1.3	220	5.5	2343	349	233	8.02	0.1	0.2	0.1
2,4'-DDE	83.5	91.3	85.6	12.5	12.9	12.1	87	4.6	12.5	3.2	78.4	9.3	14.2	1.39	0.4	0.6	0.3
4,4'-DDE	6315	6193	6287	462	467	481	6265	1.0	470	2.1	7056	981	497	19.5	-0.4	-0.5	0.1
2,4'-DDD	73.0	71.1	76.5	18.1	18.1	17.6	74	3.7	17.9	1.6	96.6	28	19.5	1.18	-1.0	-0.5	0.2
4,4'-DDD	481	456	477	130	126	122	471	2.8	126	3.2	1286	255	120	4.87	-2.5	-2.0	0.2
HCB	269	277	254	31.4	27.1	27.3	267	4.4	28.6	8.5	267	23	30.6	1.45	0.0	0.0	0.3
α -HCH	<20	<20	<20	<20	<20	<20	<20		<20		4.12	1.2	16.9	1.41			
β -HCH	<10	<10	<10	<10	<10	<10	<10		<10								
γ -HCH	<10	<10	<10	<10	<10	<10	<10		<10		2.12	2.5	3.2	0.01			
Heptachlor Epoxide	45.9	49.2	51.4	10.3	10.4	11.5	48.8	5.7	10.7	6.2	49.2	18	10.7	0.09	0.0	0.0	0.4
Cis-Chlordane	80.3	90.1	91.7	47.3	46.8	47.3	87.4	7.1	47.1	0.6	49.4	18	48.1	1.58	3.1	1.5	0.5
Trans-Chlordane	20.4	19.5	19.7	12.3	11.8	11.3	19.9	2.4	11.8	4.2	7.79	6.9	11.8	0.54	6.2	1.5	0.2
Oxychlordane	366	347	338	21.9	22.1	20.7	350	4.1	21.6	3.5	258	33	21.2	1.06	1.4	1.7	0.3
Cis-Nonachlor	237	234	224	48.3	48.5	47.3	232	2.9	48.0	1.3	232	12	45.8	3.29	0.0	0.0	0.2
Trans-Nonachlor	1916	1896	1851	193	196	190	1888	1.8	193	1.6	1494	150	198	15.5	1.1	1.7	0.1
Dieldrin	166	186	174	52.9	51.3	55.9	175	5.7	53.4	4.4	175	53	50.1	4.05	0.0	0.0	0.4
Mirex	168	164	164	28.6	27.3	27.1	165	1.4	27.7	2.9	177	24	31.0	3.35	-0.3	-0.4	0.1
PBDE 47											132	17	39.6	0.18			
PBDE 99											22.2	2.8	18.9	2.32			
PBDE 100											39.7	6.1	10.3	1.13			
PBDE 153											14.2	1.6	8.3	0.55			
PBDE 154											36.7	7.5	13.3	1.73			
Lipid (mass fraction (%))	78.8	80.3	80.1	72.5	70.8	73.1	79.7	1.05	72.2	1.63	80.5	3.3	71.9	1.27	0.0	-0.1	0.07

^aCertified values are in bold^bSee text for explanation

Category	Number by Category			
	z (25%)		z (s)	
	≤ 2	2 to 3	≥ 3	
	12	1	3	z (25%)
	15	1	0	z (s)
	16	0	0	p (15%)

PCB CONGENER ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)									Material Reference Values (ng/g wet mass)					Performance Scores ^a		
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		z-score (25%)	Homog VII z-score (s)	p-score (15%)
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	Uncert			
18	4.88	4.71	4.66	4.99	4.71	4.74	4.75	2	4.8	3.2	6.57	12.6	4.35	0.56	-1.1	-0.1	0.2
28	18.4	18.3	19.1	12.9	12.1	12.6	18.6	2.3	12.5	3.2	18.6	2.4	13.06	1.07	0.0	0.0	0.2
31	1.74	1.83	1.71	3.2	3.2	3.4	1.8	3.5	3.3	3.0	1.76	0.7	3.56	0.36	0.0	0.0	0.2
44	40.3	46.2	44.6	11.2	10.6	11.9	43.7	7.0	11.2	5.8	46.2	3.1	12.1	0.51	-0.2	-0.6	0.5
49	87.2	89.9	90.1	18.7	17.5	18.6	89.1	1.8	18.3	3.6	88.7	7.0	18.3	0.04	0.0	0.0	0.1
52	283	298	271	41.2	44.4	40.9	284	4.8	42.2	4.6	271	20	40.7	1.30	0.2	0.4	0.3
66/95*	below	below	below	below	below	below	below		below								
87	214	226	237	19.6	18.3	18.4	226	5.1	18.8	3.9	201	18	20.6	2.55	0.5	1.5	0.3
99	470	438	472	55.4	58.2	55.9	460	4.1	56.5	2.6	465	40	58.5	5.17	0.0	-0.1	0.3
101 (+90)	711	725	710	70.7	71.5	72.7	715	1.2	71.6	1.4	649	129	78.2	12.4	0.4	0.4	0.1
105	95.9	98.7	92.7	26.8	25.4	27.3	95.8	3.1	26.5	3.7	90	16	28.6	1.16	0.2	0.2	0.2
118	697	710	677	78.7	70.4	76.5	695	2.4	75.2	5.7	640	51	76.5	2.87	0.3	0.7	0.2
128	159	142	144	21.8	23.4	23.4	148	6.3	22.9	4.0	150	8.6	23.0	1.06	-0.1	-0.1	0.4
132	w/153	w/153	w/153	w/153	w/153	w/153	w/153		w/153								
138 (+163+164)	1347	1385	1394	148	134	146	1375	1.8	143	5.3	1377	136	146	12.9	0.0	0.0	0.1
149	742	762	724	97.1	97.3	90.6	743	2.6	95	4.0	741	47	89.0	6.94	0.0	0.0	0.2
151	264	232	257	27.3	26.4	26.7	251	6.7	26.8	1.7	261	20	28.6	1.33	-0.2	-0.3	0.4
153	w/132	w/132	w/132	w/132	w/132	w/132	w/132		w/132								
156	108	107	101	11.7	10.7	10.5	105	3.6	11.0	5.9	98.2	15	11.4	0.95	0.3	0.3	0.2
170 (+190)	287	298	272	44.9	42.4	42.9	286	4.6	43.4	3.0	296	16	42.6	2.18	-0.1	-0.4	0.3
180	842	821	828	133	139	127	830	1.3	133	4.5	862	75	138	9.70	-0.1	-0.2	0.1
183	243	239	216	36.9	36.2	32.1	233	6.3	35.1	7.4	234	13	38.0	1.83	0.0	-0.1	0.4
187	803	798	781	116	119	103	794	1.5	113	7.5	710	72	121	11.1	0.5	0.7	0.1
194	127	118	119	48.7	43.2	49.7	121	4.1	47.2	7.4	127	15	53.5	5.18	-0.2	-0.3	0.3
195	41.9	42.3	40.4	12.5	12.4	12.9	41.5	2.4	12.6	2.1	36.8	14	14.3	2.17	0.5	0.2	0.2
201	48.6	47.6	45.3	16.4	16.6	15.7	47.2	3.6	16.2	2.9	46.2	4.1	16.8	1.30	0.1	0.2	0.2
206	82.6	81.9	80.7	45.1	42.5	43.9	81.7	1.2	43.8	3.0	81.7	13	44.9	4.23	0.0	0.0	0.1
209	28.3	26.7	24.8	18.2	18.6	19.8	26.6	6.6	18.9	4.4	26.0	5.7	17.2	1.86	0.1	0.1	0.4
66	81.8	83.7	83.9	22.6	23.1	23.1	83.1	1.4	22.9	1.3	77.2	40	22.4	0.51	0.3	0.1	0.1
95	364	308	327	34.6	33.7	32.1	333	8.6	33.5	3.8	308	31	33.9	0.51	0.3	0.6	0.6

^aCertified values are in bold ^bSee text for explanation

Category	Number by Category		
	z (25%)	z (s)	p (15%)
≤ 2	27	27	27
2 to 3	0	0	0
≥ 3	0	0	0

PESTICIDE, PBDE, AND LIPID ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)										Material Reference Values (ng/g wet mass)				Performance Scores ^a		
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		Homog VII	Homog VII	
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	Uncert	z-score (25%)	z-score (s)	p-score (15%)
2,4'-DDT	1458	1495	1466	132	140	130	1473	1.3	134	3.9	428	243	90.9	13.5	9.8	3.4	0.09
4,4'-DDT	2471	2563	2499	245	236	237	2511	1.9	239	2.1	2343	349	233	8.02	0.3	0.3	0.13
2,4'-DDE	80.2	80.9	79.8	10.4	12.3	10.5	80.3	0.7	11.1	9.7	78.4	9.3	14.2	1.39	0.1	0.1	0.05
4,4'-DDE	10303	9566	9912	786	980	787	9927	3.7	851	13.1	7056	981	497	19.5	1.6	1.7	0.25
2,4'-DDD	83.4	86.4	84.9	20.7	22.5	20.5	84.9	1.8	21.2	5.2	96.6	28	19.5	1.18	-0.5	-0.3	0.12
4,4'-DDD	457	472	462	85.2	87.8	87.2	464	1.6	86.7	1.6	1286	255	120	4.87	-2.6	-2.0	0.11
HCB	283	272	277	33.4	29.0	35.5	277	2.0	32.6	10.2	267	23	30.6	1.45	0.2	0.3	0.13
α -HCH	<15	<15	<15	<38	<38	<38	<15		<15		4.12	1.2	16.9	1.41			
β -HCH	<7	<7	<7	<7	<7	<7	<7		<7								
γ -HCH	<7	<7	<7	<7	<7	<7	<7		<7		2.12	2.5	3.18	0.01			
Heptachlor Epoxide	49.2	50.5	49.1	9.36	12.1	9.40	49.6	1.6	10.3	15.1	49.2	18	10.7	0.09	0.0	0.0	0.10
Cis-Chlordane	92.6	95.1	92.6	77.7	87.8	77.9	93.4	1.5	81.1	7.1	49.4	18	48.1	1.58	3.6	1.7	0.10
Trans-Chlordane				5.23	6.22	5.49			5.65	9.1	7.79	6.9	11.8	0.54			
Oxychlordane	320	321	321	21.4	27.4	22.5	321	0.2	23.8	13.4	258	33	21.2	1.06	1.0	1.2	0.01
Cis-Nonachlor	237	246	242	53.6	55.6	55.7	242	1.9	55.0	2.2	232	12	45.8	3.29	0.2	0.6	0.12
Trans-Nonachlor	1855	1848	1850	240	249	234	1851	0.2	241	3.1	1494	150	198	15.5	1.0	1.5	0.01
Dieldrin	211	217	197	50.9	57.3	49.3	208	4.9	52.5	8.1	175	53	50.1	4.05	0.8	0.5	0.33
Mirex	178	176	177	37.3	38.4	36.6	177	0.6	37.4	2.4	177	24	31.0	3.35	0.0	0.0	0.04
PBDE 47									132	17	39.6	0.18					
PBDE 99									22.2	2.8	18.9	2.32					
PBDE 100									39.7	6.1	10.3	1.13					
PBDE 153									14.2	1.6	8.3	0.55					
PBDE 154									36.7	7.5	13.3	1.73					
Lipid (mass fraction (%))	76.9	100	103	64.4	64.2	87.4	93.5	15.5	72.0	18.5	80.5	3.3	71.9	1.27	0.6	1.8	1.04

^aCertified values are in bold^bSee text for explanation

Category	Number by Category		
	z (25%)	z (s)	p (15%)
	≤ 2	2 to 3	≥ 3
	12	14	15
	1	0	0
	2	1	0
	z (25%)	z (s)	p (15%)

PCB CONGENER ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)									Material Reference Values (ng/g wet mass)				Performance Scores ^a			
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		z-score	Homog VII	z-score
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	95% CL	(25%)	(s)	(15%)
18	3.44	3.25	3.68	3.15	3.50	3.81	3.46	6	3.49	9.5	6.57	12.6	4.35	0.56	-1.9	-0.2	0.42
28	19.4	17.9	18.3	9.9	9.2	10.7	18.5	4.2	9.91	7.7	18.6	2.4	13.06	1.07	0.0	0.0	0.28
31	<1	<1	<1	3.7	4.0	4.1	<1		3.94	5.0	1.76	0.7	3.56	0.36			
44	46.5	43.6	43.7	11.3	10.7	11.8	44.6	3.7	11.3	5.1	46.2	3.1	12.1	0.51	-0.1	-0.4	0.25
49	88.5	84.0	85.4	18.5	17.1	20.0	86.0	2.7	18.5	7.7	88.7	7.0	18.3	0.04	-0.1	-0.3	0.18
52	284	270	273	40.5	37.7	41.1	276	2.7	39.8	4.5	271	20	40.7	1.30	0.1	0.1	0.18
66/95*	below	below	below	below	below	below	below										
87	222	222	217	26.9	29.7	28.1	220	1.3	28.2	5.1	201	18	20.6	2.55	0.4	1.2	0.09
99	495	496	479	66.4	71.9	66.4	490	1.9	68.2	4.7	465	40	58.5	5.17	0.2	0.4	0.13
101 (+90)	762	758	739	101	112	99.5	753	1.6	104	6.5	649	129	78.2	12.4	0.6	0.6	0.11
105	96.8	96.4	93.9	29.6	32.4	30.3	95.7	1.6	30.8	4.7	90	16	28.6	1.16	0.2	0.2	0.11
118	710	716	686	95.9	104.6	96.3	704	2.3	98.9	5.0	640	51	76.5	2.87	0.4	0.8	0.15
128	157	159	155	24.4	26.2	23.7	157	1.3	24.8	5.2	150	8.6	23.0	1.06	0.2	0.5	0.08
132	w/153	w/153	w/153	w/153	w/153	w/153	w/153						21.1	4.75			
138 (+163+164)	1398	1387	1378	163	176	161	1388	0.7	166	5.1	1377	136	146	12.9	0.0	0.0	0.05
149	767	767	749	97.2	104.4	96.1	761	1.4	99.2	4.5	741	47	89.0	6.94	0.1	0.2	0.09
151	278	278	275	31.8	34.8	30.9	277	0.6	32.5	6.2	261	20	28.6	1.33	0.2	0.5	0.04
153	2550	2531	2521	327	353	323	2534	0.6	334	4.8	1831	240	228	9.75	1.5	2.2	0.04
156	100	105	101	13.7	14.6	13.7	102	2.6	14.0	3.9	98.2	15	11.4	0.95	0.2	0.2	0.17
170 (+190)	299	305	299	45.5	49.2	46.0	301	1.2	46.9	4.3	296	16	42.6	2.18	0.1	0.2	0.08
180	897	922	907	165	174	168	909	1.4	169	2.6	862	75	138	9.70	0.2	0.4	0.09
183	256	255	252	44.0	46.5	43.5	254	0.8	44.7	3.6	234	13	38.0	1.83	0.3	0.9	0.05
187	802	801	797	143	151	143	800	0.3	146	3.1	710	72	121	11.1	0.5	0.8	0.02
194	127	128	125	60.0	61.7	59.2	127	1.2	60.3	2.1	127	15	53.5	5.18	0.0	0.0	0.08
195	36.0	36.0	35.3	11.4	12.1	11.0	35.8	1.1	11.5	4.6	36.8	14	14.3	2.17	-0.1	0.0	0.08
201	44.7	45.5	45.3	15.5	16.4	15.6	45.2	0.9	15.8	3.1	46.2	4.1	16.8	1.30	-0.1	-0.2	0.06
206	84.1	85.5	84.3	53.4	55.5	54.1	84.6	0.9	54.3	1.9	81.7	13	44.9	4.23	0.1	0.2	0.06
209	26.2	25.1	24.6	20.2	20.5	20.7	25.3	3.2	20.5	1.3	26.0	5.7	17.2	1.86	-0.1	-0.1	0.22
66	78.1	77.5	75.9	25.6	28.0	26.5	77.2	1.5	26.7	4.4	77.2	40	22.4	0.51	0.0	0.0	0.10
95	362	361	349	46.4	51.6	45.8	357	2.0	47.9	6.6	308	31	33.9	0.51	0.6	1.3	0.13

^aCertified values are in bold ^bSee text for explanation

Category	Number by Category		
	z (25%)	z (s)	p (15%)
≤ 2	27	26	27
2 to 3	0	1	0
≥ 3	0	0	0

PESTICIDE, PBDE, AND LIPID ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)								Material Reference Values (ng/g wet mass)				Performance Scores ^a				
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		Homog VII		
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	Uncert	z-score (25%)	z-score (s)	p-score (15%)
2,4'-DDT	424	439	437	57.5			433	1.9	58		428	243	90.9	13.5	0.1	0.0	0.13
4,4'-DDT	2240	2300	2420	169			2320	4.0	169		2343	349	233	8.02	0.0	0.0	0.26
2,4'-DDE	75.4	76.9	77.4	14.2			76.6	1.4	14.2		78.4	9.3	14.2	1.39	-0.1	-0.1	0.09
4,4'-DDE	7660	7590	7730	516			7660	0.9	516		7056	981	497	19.5	0.3	0.3	0.06
2,4'-DDD	92.1	98.2	99.6	18.5			96.6	4.1	18.5		96.6	28	19.5	1.18	0.0	0.0	0.28
4,4'-DDD	1270	1340	1360	117			1323	3.6	117.0		1286	255	120	4.87	0.1	0.1	0.24
HCB	252	249	252	27.3			251	0.7	27.3		267	23	30.6	1.45	-0.2	-0.4	0.05
α-HCH	4.44	4.74	<2.49	16.1			4.59	4.6	16		4.12	1.2	16.9	1.41	0.5	0.4	0.31
β-HCH	3.88	2.66	<2.47	5.02			3.27	26.4	5								
γ-HCH	<2.16	<1.79	<2.37	2.95					3		2.12	2.5	3.18	0.01			
Heptachlor Epoxide	55.1	59.0	63.5	10.00			59.2	7.1	10.0		49.2	18	10.7	0.09	0.8	0.5	0.47
Cis-Chlordane	28.3	34.9	32.9	51.0			32.0	10.6	51.0		49.4	18	48.1	1.58	-1.4	-0.7	0.70
Trans-Chlordane	7.15	7.91	7.80	11.20			7.6	5.4	11.20		7.79	6.9	11.8	0.54	-0.1	0.0	0.36
Oxychlordane	260	268	267	17.4			265	1.6	17.4		258	33	21.2	1.06	0.1	0.1	0.11
Cis-Nonachlor	246	257	264	50.7			256	3.5	50.7		232	12	45.8	3.29	0.4	1.5	0.24
Trans-Nonachlor	1390	1410	1430	162			1410	1.4	162		1494	150	198	15.5	-0.2	-0.4	0.09
Dieldrin	206	212	213	47.6			210	1.8	47.6		175	53	50.1	4.05	0.8	0.5	0.12
Mirex	183	186	192	32.6			187	2.5	32.6		177	24	31.0	3.35	0.2	0.4	0.16
PBDE 47	147	156	157	37.0			153	3.6	37		132	17	39.6	0.18	0.6	0.9	0.24
PBDE 99	24.7	26.5	27.8	15			26.3	5.9	15		22.2	2.8	18.9	2.32	0.7	1.3	0.39
PBDE 100	37.1	41.3	40.7	8.4			39.7	5.7	8		39.7	6.1	10.3	1.13	0.0	0.0	0.38
PBDE 153	14.7	15.4	16.0	7.5			15.4	4.2	7		14.2	1.6	8.34	0.55	0.3	0.6	0.28
PBDE 154	35.7	38.2	38.5	11.3			37.5	4.1	11		36.7	7.5	13.3	1.73	0.1	0.1	0.27
Lipid (mass fraction (%))	71.7	69.3	70.6	61.9			70.5	1.7	61.9		80.5	3.3	71.9	1.27	-0.5	-1.3	0.11

^aCertified values are in bold^bSee text for explanation

Category	Number by Category		
	z (25%)	z (s)	p (15%)
	≤ 2	2 to 3	≥ 3
	22	22	22
	0	0	0
	0	0	0
	z (25%)	z (s)	p (15%)

PCB CONGENER ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)									Material Reference Values (ng/g wet mass)				Performance Scores ^a			
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		Homog VII	z-score	
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	Uncert	(s)	p-score (15%)	
18																	
28	16.2	15.7	13.9	10.5			15.3	7.9	10.50		18.6	2.4	13.06	1.07	-0.7	-0.9	0.53
31	2.79	2.80	2.48	3.23			2.69	6.8	3.23		1.76	0.7	3.56	0.36	2.1	1.4	0.45
44	48.3	48.1	49.0	12.8			48.5	1.0	12.8		46.2	3.1	12.1	0.51	0.2	0.5	0.07
49	89.3	91.9	97.0	18.8			92.7	4.2	18.8		88.7	7.0	18.3	0.04	0.2	0.4	0.28
52	269	268	271	38.1			269	0.6	38.1		271	20	40.7	1.30	0.0	-0.1	0.04
66/95*	na	na	na	na			na										
87	198	200	204	26.0			201	1.5	26.0		201	18	20.6	2.55	0.0	0.0	0.10
99	423	428	426	56.8			426	0.6	56.8		465	40	58.5	5.17	-0.3	-0.6	0.04
101 (+90)	607	609	610	78			609	0.3	78.2		649	129	78.2	12.4	-0.2	-0.2	0.02
105	88.7	84.2	76.1	28.1			83.0	7.7	28.1		90	16	28.6	1.16	-0.3	-0.3	0.51
118	664	671	676	84.5			670	0.9	84.5		640	51	76.5	2.87	0.2	0.4	0.06
128	153	155	158	23.7			155	1.6	23.7		150	8.6	23.0	1.06	0.1	0.4	0.11
132	na	na	na	na			na		n				21.1	4.75			
138 (+163+164)	1560	1550	1580	189			1563	1.0	189		1377	136	146	12.9	0.5	0.8	0.07
149	731	746	747	84.1			741	1.2	84.1		741	47	89.0	6.94	0.0	0.0	0.08
151	257	260	265	27.8			261	1.6	27.8		261	20	28.6	1.33	0.0	0.0	0.10
153	1960	1950	2000	249			1970	1.3	249		1831	240	228	9.75	0.3	0.4	0.09
156	91.5	94.8	96.8	12.3			94	2.8	12.3		98.2	15	11.4	0.95	-0.2	-0.2	0.19
170 (+190)											296	16	42.6	2.18			
180	824	829	848	143			834	1.5	143		862	75	138	9.70	-0.1	-0.2	0.10
183	233	234	241	39.9			236	1.8	39.9		234	13	38.0	1.83	0.0	0.1	0.12
187	710	725	724	116			720	1.2	116		710	72	121	11.1	0.1	0.1	0.08
194	125	128	130	55.7			128	2.0	55.7		127	15	53.5	5.18	0.0	0.0	0.13
195	33.2	33.7	34.3	10.3			33.7	1.6	10.3		36.8	14	14.3	2.17	-0.3	-0.1	0.11
201	271	278	279	80.2			276.0	1.6	80.2		46.2	4.1	16.8	1.30	19.9	55.1	0.11
206	77.9	80.1	80.0	48.5			79.3	1.6	48.5		81.7	13	44.9	4.23	-0.1	-0.1	0.10
209	23.6	24.1	24.1	18.1			23.9	1.2	18.1		26.0	5.7	17.2	1.86	-0.3	-0.2	0.08
66	72.1	75.1	73.0	22.2			73.4	2.1	22.2		77.2	40	22.4	0.51	-0.2	-0.1	0.14
95	330	337	338	39.6			335	1.3	39.6		308	31	33.9	0.51	0.4	0.7	0.09

^aCertified values are in bold ^bSee text for explanation

Category	Number by Category		
	z (25%)	z (s)	p (15%)
	≤ 2	2 to 3	≥ 3
24	25	26	
1	0	0	
1	1	0	

SAMPLES: Homogenate VII AND SRM 1945

PESTICIDE, PBDE, AND LIPID ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)										Material Reference Values (ng/g wet mass)				Performance Scores ^a		
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		Homog VII	Homog VII	
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	Uncert	z-score (25%)	z-score (s)	p-score (15%)
2,4'-DDT	333	336	330	85.9	90.9	79.4	333	0.9	85.4	6.8	428	243	90.9	13.5	-0.9	-0.3	0.06
4,4'-DDT	2350	2360	2320	231	233	222	2343	0.9	229	2.6	2343	349	233	8.02	0.0	0.0	0.06
2,4'-DDE									78.4	9.3	14.2	1.39					
4,4'-DDE	8610	8610	8670	484	459	488	8630	0.4	477	3.3	7056	981	497	19.5	0.9	0.9	0.03
2,4'-DDD	118	131	127	25.4	25.6	23.0	125	5.3	24.7	5.9	96.6	28	19.5	1.18	1.2	0.7	0.35
4,4'-DDD	1460	1480	1480	116	112	113	1473	0.8	114	1.8	1286	255	120	4.87	0.6	0.5	0.05
HCB	308	318	316	30.6	31.4	29.9	314	1.7	30.6	2.5	267	23	30.6	1.45	0.7	1.3	0.11
α -HCH									4.12	1.2	16.9	1.41					
β -HCH									2.12	2.5	3.18	0.01					
γ -HCH									49.2	18	10.7	0.09					
Heptachlor Epoxide									49.4	18	48.1	1.58					
Cis-Chlordane									7.79	6.9	11.8	0.54					
Trans-Chlordane									258	33	21.2	1.06					
Oxychlordane									232	12	45.8	3.29					
Cis-Nonachlor									1494	150	198	15.5					
Trans-Nonachlor									175	53	50.1	4.05					
Dieldrin									177	24	31.0	3.35					
Mirex									132	17	39.6	0.18					
PBDE 47									22.2	2.8	18.9	2.32					
PBDE 99									39.7	6.1	10.3	1.13					
PBDE 100									14.2	1.6	8.34	0.55					
PBDE 153									36.7	7.5	13.3	1.73					
PBDE 154									80.5	3.3	71.9	1.27	0.4	1.0	0.42		
Lipid (mass fraction (%))	84.0	85.2	94.1	54.1	49.7	53.4	87.7	6.29	52.4	4.50							

^aCertified values are in bold^bSee text for explanation

Category	Number by Category		
	z (25%)	z (s)	p (15%)
≤ 2	7	7	7
2 to 3	0	0	0
≥ 3	0	0	0
	z (25%)	z (s)	p (15%)

PCB CONGENER ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)									Material Reference Values (ng/g wet mass)				Performance Scores ^a			
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		z-score (25%)	Homog VII z-score (s)	p-score (15%)
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	Uncert			
18											6.57	12.6	4.35	0.56			
28											18.6	2.4	13.06	1.07			
31											1.76	0.7	3.56	0.36			
44											46.2	3.1	12.1	0.51			
49											88.7	7.0	18.3	0.04			
52											271	20	40.7	1.30			
66/95*																	
87											201	18	20.6	2.55			
99											465	40	58.5	5.17			
101 (+90)	2870	2990	3000	458.0	459.0	452.0	2953	2.4	456.3	0.8	649	129	78.2	12.4	14.2	12.4	0.16
105	90.4	92.4	88.0	30.7	32.9	31.2	90.3	2.4	31.6	3.6	90.3	16	28.6	1.16	0.0	0.00	0.16
118	812	816	811	95.8	97.2	95.2	813	0.3	96.1	1.1	640	51	76.5	2.87	1.1	2.11	0.02
128	146	154	132	22.8	16.6	20.7	144	7.7	20.0	15.7	150	8.6	23.0	1.06	-0.2	-0.45	0.52
132													21.1	4.75			
138 (+163+164)	1360	1400	1370	142	146	143	1377	1.5	144	1.4	1377	136	146	12.9	0.0	0.00	0.10
149											741	47	89.0	6.94			
151											261	20	28.6	1.33			
153	2210	2250	2160	278	277	281	2207	2.0	279	0.7	1831	240	228	9.75	0.8	1.16	0.14
156	75.0	76.4	76.4	8.32	7.84	7.89	75.9	1.1	8.02	3.3	98.2	15	11.4	0.95	-0.9	-0.94	0.07
170 (+190)											296	16	42.6	2.18			
180	903	858	908	142	141	139	890	3.1	141	1.1	862	75	138	9.70	0.1	0.21	0.21
183											234	13	38.0	1.83			
187											710	72	121	11.1			
194											127	15	53.5	5.18			
195											37	14	14.3	2.17			
201											46.2	4.1	16.8	1.30			
206											81.7	13	44.9	4.23			
209											26.0	5.7	17.2	1.86			
66											77.2	40	22.4	0.51			
95											308	31	33.9	0.51			
													Number by Category				
													Category	z (25%)	z (s)	p (15%)	
													≤ 2	7	6	8	
													2 to 3	0	1	0	
													≥ 3	1	1	0	

^aCertified values are in bold ^bSee text for explanation

PESTICIDE, PBDE, AND LIPID ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)										Material Reference Values (ng/g wet mass)				Performance Scores ^a		
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		Homog VII	Homog VII	
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	Uncert	z-score (25%)	z-score (s)	p-score (15%)
2,4'-DDT	290	295	301	91.8	75.3	88.8	295	1.9	85.3	10.3	428	243	90.9	13.5	-1.2	-0.4	0.13
4,4'-DDT	1427	1389	1481	196	193	200	1432	3.2	196	1.8	2343	349	233	8.02	-1.6	-1.7	0.21
2,4'-DDE	73.3	72.4	72.9	16.4	18.5	17.3	72.9	0.6	17.4	6.1	78.4	9.3	14.2	1.39	-0.3	-0.4	0.04
4,4'-DDE	6581	6534	6446	491	479	477	6520	1.1	482	1.5	7056	981	497	19.5	-0.3	-0.3	0.07
2,4'-DDD	113	114	104	56.0	54.5	49.1	110	4.8	53.2	6.8	96.6	28	19.5	1.18	0.6	0.3	0.32
4,4'-DDD	1093	1092	1042	155	156	144	1076	2.7	152	4.3	1286	255	120	4.87	-0.7	-0.5	0.18
HCB	291	290	284	43.3	40.7	39.8	288	1.3	41.3	4.4	267	23	30.6	1.45	0.3	0.6	0.09
α -HCH	<0.74	<0.74	<0.74	<0.74	<0.74	<0.74	<0.74		<0.74		4.12	1.2	16.9	1.41			
β -HCH	<0.64	<0.64	<0.64	<0.64	<0.64	<0.64	<0.64		<0.64								
γ -HCH	<2.47	<2.47	<2.47	<2.47	<2.47	<2.47	<2.47		<2.47		2.12	2.5	3.2	0.01			
Heptachlor Epoxide	63.7	64.5	63.3	24.6	24.7	22.4	63.8	0.9	23.9	5.4	49.2	18	10.7	0.09	1.2	0.8	0.06
Cis-Chlordane	31.6	27.9	29.6	45.1	44.5	40.8	29.7	6.1	43.5	5.4	49.4	18	48.1	1.58	-1.6	-0.8	0.41
Trans-Chlordane	7.14	7.05	7.24	11.0	11.1	11.1	7.14	1.3	11.1	0.4	7.79	6.9	11.8	0.54	-0.3	-0.1	0.09
Oxychlordane	237	239	244	18.5	18.7	19.0	240	1.5	18.7	1.4	258	33	21.2	1.06	-0.3	-0.4	0.10
Cis-Nonachlor	199	198	196	61.2	62.4	63.8	198	0.9	62.5	2.0	232	12	45.8	3.29	-0.6	-2.1	0.06
Trans-Nonachlor	1502	1469	1512	173	173	173	1494	1.5	173	0.1	1494	150	198	15.5	0.0	0.0	0.10
Dieldrin	237	232	237	58.0	72.2	70.8	235	1.2	67.0	11.6	175	53	50.1	4.05	1.4	0.8	0.08
Mirex	128	128	128	39.5	40.0	39.0	128	0.2	39.5	1.2	177	24	31.0	3.35	-1.1	-1.8	0.01
PBDE 47	173	173	175	51.8	47.8	54.9	174	0.7	51.5	6.9	132	17	39.6	0.18	1.2	1.7	0.04
PBDE 99	44.4	43.0	43.1	29.3	28.0	31.0	43.5	1.8	29.4	5.2	22.2	2.8	18.9	2.32	3.8	6.7	0.12
PBDE 100	45.2	44.3	44.9	16.6	16.3	16.4	44.8	1.0	16.4	1.2	39.7	6.1	10.3	1.13	0.5	0.6	0.07
PBDE 153	26.7	26.2	25.6	16.1	17.0	18.7	26.1	2.1	17.3	7.8	14.2	1.6	8.3	0.55	3.3	6.0	0.14
PBDE 154	63.0	60.0	61.7	33.3	31.0	28.2	61.6	2.4	30.8	8.3	36.7	7.5	13.3	1.73	2.7	2.6	0.16
Lipid (mass fraction (%))	81.0	82.0	82.0	67.0	69.4	70.0	81.7	0.71	68.8	2.31	80.5	3.3	71.9	1.27	0.1	0.2	0.05

^aCertified values are in bold^bSee text for explanation

PCB CONGENER ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)										Material Reference Values (ng/g wet mass)				Performance Scores ^a		
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		z-score	Homog VII	z-score
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	Uncert	(25%)	(s)	(15%)
18	8.79	7.84	8.56	7.82	9.81	7.65	8.40	6	8.4	14.3	6.57	12.6	4.35	0.56	1.1	0.14	0.39
28											18.6	2.4	13.06	1.07			
31											1.76	0.7	3.56	0.36			
44	47.9	47.8	47.4	17.1	17.4	16.2	47.7	0.6	16.9	3.8	46.2	3.1	12.1	0.51	0.1	0.36	0.04
49	97.7	96.3	96.0	28.6	29.9	26.3	96.7	1.0	28.3	6.4	88.7	7.0	18.3	0.04	0.4	0.84	0.06
52	222	221	222	37.4	36.4	35.1	222	0.3	36.3	3.2	271	20	40.7	1.30	-0.7	-1.47	0.02
66/95*																	
87											201	18	20.6	2.55			
99	478	467	487	71.1	68.6	69.4	477	2.1	69.7	1.8	465	40	58.5	5.17	0.1	0.18	0.14
101 (+90)											649	129	78.2	12.4			
105	77.0	74.5	77.0	31.7	31.7	29.7	76.1	1.9	31.0	3.8	90	16	28.6	1.16	-0.6	-0.52	0.13
118											640	51	76.5	2.87			
128											150	8.6	23.0	1.06			
132													21.1	4.75			
138 (+163+164)											1377	136	146	12.9			
149	860	843	875	98.9	98.4	97.7	859	1.9	98.3	0.6	741	47	89.0	6.94	0.6	1.47	0.12
151	264	256	267	32.2	32.0	31.1	262	2.3	31.7	1.8	261	20	28.6	1.33	0.0	0.03	0.15
153											1831	240	228	9.75			
156	90.5	91.2	90.2	15.2	16.6	15.7	90.6	0.6	15.8	4.7	98.2	15	11.4	0.95	-0.3	-0.32	0.04
170 (+190)	275	300	297	47.4	47.7	46.1	291	4.6	47.1	1.8	296	16	42.6	2.18	-0.1	-0.21	0.31
180	790	820	790	140	144	140	800	2.1	141	1.8	862	75	138	9.70	-0.3	-0.46	0.14
183	189	199	208	37.6	37.0	37.4	199	4.9	37.4	0.8	234	13	38.0	1.83	-0.6	-1.67	0.32
187	619	648	678	118	116	118	648	4.5	117	0.7	710	72	121	11.1	-0.3	-0.52	0.30
194	148	150	149	79.8	84.5	72.0	149	0.6	78.8	8.0	127	15	53.5	5.18	0.7	1.01	0.04
195	38.3	36.9	37.4	16.3	16.1	13.8	37.5	1.9	15.4	8.8	37	14	14.3	2.17	0.1	0.03	0.13
201	278	267	283	26.4	26.3	22.2	276.2	2.9	24.9	9.6	46.2	4.1	16.8	1.30	19.9	55.15	0.19
206	63.3	64.7	63.7	37.2	42.1	40.0	63.9	1.1	39.8	6.1	81.7	13	44.9	4.23	-0.9	-0.92	0.08
209	17.8	17.7	18.8	13.0	13.2	13.8	18.1	3.1	13.3	3.2	26.0	5.7	17.2	1.86	-1.2	-0.95	0.21
66	88.1	88.0	85.9	30.1	31.3	30.1	87.3	1.4	30.5	2.3	77.2	40	22.4	0.51	0.5	0.17	0.09
95	248	247	254	38.7	40.3	38.8	250	1.4	39.3	2.3	308	31	33.9	0.51	-0.8	-1.49	0.09

^aCertified values are in bold ^bSee text for explanation

Category	Number by Category		
	z (25%)	z (s)	p (15%)
	≤ 2	2 to 3	≥ 3
	19	19	20
	0	0	0
	1	1	0

SAMPLES: Homogenate VII AND SRM 1945

PESTICIDE, PBDE, AND LIPID ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)										Material Reference Values (ng/g wet mass)				Performance Scores ^a		
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		Homog VII	Homog VII	Homog VII
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	Uncert	z-score (25%)	z-score (s)	p-score (15%)
2,4'-DDT	518	531	519	96.0	103	103	523	1.4	101	4.0	428	243	90.9	13.5	0.9	0.3	0.09
4,4'-DDT	3180	3260	3240	349	370	367	3227	1.3	362	3.1	2343	349	233	8.02	1.5	1.7	0.09
2,4'-DDE	67.2	65.7	65.8	12.9	15.5	14.4	66	1.3	14.3	9.1	78.4	9.3	14.2	1.39	-0.6	-0.9	0.08
4,4'-DDE	7150	7090	7190	485	515	526	7143	0.7	509	4.2	7056	981	497	19.5	0.0	0.1	0.05
2,4'-DDD	115	115	117	23.8	26.6	25.0	116	1.0	25.1	5.6	96.6	28	19.5	1.18	0.8	0.4	0.07
4,4'-DDD											1286	255	120	4.87			
HCB	279	263	258	36.2	36.6	38.4	267	4.1	37.1	3.2	267	23	30.6	1.45	0.0	0.0	0.27
α -HCH											4.12	1.2	16.9	1.41			
β -HCH	12.7	10.4	18.4	18.4	7.15	8.09	13.8	29.8	11.2	56							
γ -HCH	19.2	14.5	17.3	102	89.0	129	17.0	13.9	107	19	2.12	2.5	3.18	0.01	28.1	8.4	0.93
Heptachlor Epoxide	52.1	52.8	48.3	16.8	20.2	16.6	51.1	4.7	17.9	11	49.2	18	10.7	0.09	0.2	0.1	0.32
Cis-Chlordane	17.6	14.9	20.9	43.5	46.3	47.2	17.8	16.9	45.7	4.2	49.4	18	48.1	1.58	-2.6	-1.2	1.13
Trans-Chlordane	31.2	9.09	10.1	20.2	20.7	19.6	16.8	74.3	20.2	2.7	7.79	6.9	11.8	0.54	4.6	1.1	4.95
Oxychlordane	250	250	255	20.2	22.8	21.4	252	1.1	21.5	6.1	258	33	21.2	1.06	-0.1	-0.1	0.08
Cis-Nonachlor											232	12	45.8	3.29			
Trans-Nonachlor	1360	1350	1370	164	173	173	1360	0.7	170	3.1	1494	150	198	15.5	-0.4	-0.6	0.05
Dieldrin											175	53	50.1	4.05			
Mirex											177	24	31.0	3.35			
PBDE 47	140	146	142	38.8	40.9	42.9	143	2.1	41	5.0	132	17	39.6	0.18	0.3	0.4	0.14
PBDE 99	27.7	26.3	25.9	16.5	18.3	17.9	26.6	3.5	18	5.4	22.2	2.8	18.9	2.32	0.8	1.4	0.24
PBDE 100	41.6	40.7	40.0	9.3	9.9	9.3	40.8	2.0	9.51	3.9	39.7	6.1	10.3	1.13	0.1	0.1	0.13
PBDE 153	17.1	15.9	15.4	6.1	8.2	7.2	16.1	5.4	7.16	14.8	14.2	1.6	8.34	0.55	0.5	1.0	0.36
PBDE 154	44.4	44.5	44.9	11.4	12.8	12.6	44.6	0.6	12.3	6.2	36.7	7.5	13.3	1.73	0.9	0.8	0.04
Lipid (mass fraction (%))	86.0	88.2	90.7	73.6	73.2	75.7	88.3	2.65	74.1	1.79	80.5	3.3	71.9	1.27	0.4	1.1	0.18

^aCertified values are in bold^bSee text for explanation

Category	Number by Category		
	z (25%)	z (s)	p (15%)
	≤ 2	2 to 3	≥ 3
	15	17	17
	1	0	0
	2	1	1
	z (25%)	z (s)	p (15%)

PCB CONGENER ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)									Material Reference Values (ng/g wet mass)				Performance Scores ^a			
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		Homog VII	z-score (s)	p-score (15%)
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	Uncert	z-score (25%)	z-score (s)	p-score (15%)
18	33.3	29.9	29.3	4.47	5.85	DL	30.8	7	5.2	18.9	6.57	12.6	4.35	0.56	14.8	1.9	0.47
28	20.8	16.1	16.2	13.5	14.1	13.8	17.7	15.2	13.8	2.2	18.6	2.4	13.06	1.07	-0.2	-0.3	1.01
31	3.52	2.74	2.80	6.24	6.36	6.66	3.02	14.4	6.42	3.4	1.76	0.7	3.56	0.36	2.9	1.9	0.96
44	56.2	54.3	55.5	13.8	12.0	13.1	55.3	1.7	13.0	7.0	46.2	3.1	12.1	0.51	0.8	2.2	0.12
49	99.4	98.3	98.6	23.2	26.4	26.2	98.8	0.6	25.3	7.1	88.7	7.0	18.3	0.04	0.5	1.1	0.04
52	274	269	267	43.2	48.9	50.4	270	1.3	47.5	8.0	271	20	40.7	1.30	0.0	0.0	0.09
66/95*	380	379	380	62.7	66.9	62.4	380	0.2	64.0	3.9							
87											201	18	20.6	2.55			
99	467	464	465	62.0	66.0	63.3	465	0.3	63.8	3.2	465	40	58.5	5.17	0.0	0.0	0.02
101 (+90)											649	129	78.2	12.4			
105	111	113	113	36.5	39.0	37.5	112	1.0	37.7	3.3	90	16	28.6	1.16	1.0	0.8	0.07
118	635	632	640	83.1	91.5	89.8	636	0.6	88.1	5.0	640	51	76.5	2.87	0.0	-0.1	0.04
128	159	157	156	34.6	36.1	33.7	157	1.0	34.8	3.5	150	8.6	23.0	1.06	0.2	0.5	0.06
132													21.1	4.75			
138 (+163+164)	1230	1220	1200	165	173	158	1217	1.3	165	4.5	1377	136	146	12.9	-0.5	-0.7	0.08
149	703	693	695	92.9	98.8	94.7	697	0.8	95.5	3.2	741	47	89.0	6.94	-0.2	-0.6	0.05
151	278	275	279	31.6	33.3	31.7	277	0.8	32.2	3.0	261	20	28.6	1.33	0.2	0.5	0.05
153	1380	1410	1370	200	214	189	1387	1.5	201	6.2	1831	240	228	9.75	-1.0	-1.4	0.10
156	103.0	101.0	103.0	14.4	15.5	14.0	102.3	1.1	14.6	5.3	98.2	15	11.4	0.95	0.2	0.2	0.08
170 (+190)	297	272	273	39.0	43.0	39.0	281	5.0	40.3	5.7	296	16	42.6	2.18	-0.2	-0.6	0.34
180	841	823	818	164	172	158	827	1.5	165	4.3	862	75	138	9.70	-0.2	-0.3	0.10
183	263	259	255	49.3	51.8	47.3	259	1.5	49.5	4.6	234	13	38.0	1.83	0.4	1.2	0.10
187	641	637	626	130	138	123	635	1.2	130	5.8	710	72	121	11.1	-0.4	-0.6	0.08
194	166	159	157	77.4	80.9	75.4	161	2.9	77.9	3.6	127	15	53.5	5.18	1.1	1.5	0.20
195	78.9	76.9	75.3	12.1	12.1	10.5	77.0	2.3	11.6	8.0	37	14	14.3	2.17	4.4	1.9	0.16
201	284.0	266.0	265.0	87.6	91.8	83.2	272	3.9	87.5	4.9	46.2	4.1	16.8	1.30	19.5	54.1	0.26
206	85.3	84.3	83.6	51.1	54.5	49.7	84.4	1.0	51.8	4.8	81.7	13	44.9	4.23	0.1	0.1	0.07
209	34.4	35.4	35.3	26.1	26.1	24.4	35.0	1.6	25.5	3.8	26.0	5.7	17.2	1.86	1.4	1.1	0.10
66											77.2	40	22.4	0.51			
95											308	31	33.9	0.51			
Number by Category																	
Category		z (25%)			z (s)			p (15%)									
≤ 2		20			22			24									
2 to 3		1			1			0									
≥ 3		3			1			0									

^aCertified values are in bold ^bSee text for explanation

SAMPLES: Homogenate VII AND SRM 1945

PESTICIDE, PBDE, AND LIPID ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)										Material Reference Values (ng/g wet mass)				Performance Scores ^a		
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		Homog VII	Homog VII	Homog VII
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	Uncert	z-score (25%)	z-score (s)	p-score (15%)
2,4'-DDT	1020	873	1140	134.0	122	136	1011	13.2	131	5.8	428	243	90.9	13.5	5.5	1.9	0.88
4,4'-DDT	3380	2710	3420	251	250	253	3170	12.6	251	0.6	2343	349	233	8.02	1.4	1.5	0.84
2,4'-DDE	86.2	74.2	86.9	13.4	14.5	14.7	82	8.7	14.2	4.9	78.4	9.3	14.2	1.39	0.2	0.3	0.58
4,4'-DDE	10800	9710	10600	687	694	679	10370	5.6	687	1.1	7056	981	497	19.5	1.9	1.9	0.37
2,4'-DDD	190	190	213	22.0	23.0	20.2	198	6.7	21.7	6.5	96.6	28	19.5	1.18	4.2	2.4	0.45
4,4'-DDD	2750	2190	2530	198	197	202	2490	11.3	199	1.3	1286	255	120	4.87	3.7	2.9	0.76
HCB	286	274	277	28.4	30.0	31.3	279	2.2	29.9	4.9	267	23	30.6	1.45	0.2	0.3	0.15
α-HCH	6.63	5.50	6.61	17.6	18.2	16.9	6.25	10	17.6	3.7	4.12	1.2	16.9	1.41	2.1	1.7	0.69
β-HCH				7.72	10.1	13.5			10.4	28							
γ-HCH	5.06	5.91	5.86	6.30	11.6	7.12	5.61	8.5	8.34	34	2.12	2.5	3.18	0.01	6.6	2.0	0.57
Heptachlor Epoxide				11.2	27.6	7.34			15.4	70	49.2	18	10.7	0.09			
Cis-Chlordane	54.5	43.2	45.6	49.6	48.7	52.4	47.8	12.5	50.2	3.8	49.4	18	48.1	1.58	-0.1	-0.1	0.83
Trans-Chlordane	45.9	36.2	41.5	26.2	25.5	29.4	41.2	11.8	27.0	7.7	7.79	6.9	11.8	0.54	17.1	4.2	0.79
Oxychlordane	203	264	228	24.1	24.3	25.9	232	13.2	24.8	4.0	258	33	21.2	1.06	-0.4	-0.5	0.88
Cis-Nonachlor	268	219	256	52.8	49.8	56.4	248	10.3	53.0	6.2	232	12	45.8	3.29	0.3	1.0	0.69
Trans-Nonachlor	1490	1280	1420	192	195	205	1397	7.7	197	3.4	1494	150	198	15.5	-0.3	-0.4	0.51
Dieldrin	313	313	284	58.1	59.5	58.9	303	5.5	58.8	1.2	175	53	50.1	4.05	2.9	1.8	0.37
Mirex	245	220	246	42.1	43.6	43.2	237	6.2	43.0	1.8	177	24	31.0	3.35	1.4	2.2	0.41
PBDE 47									132	17	39.6	0.18					
PBDE 99									22.2	2.8	18.9	2.32					
PBDE 100									39.7	6.1	10.3	1.13					
PBDE 153									14.2	1.6	8.34	0.55					
PBDE 154									36.7	7.5	13.3	1.73					
Lipid (mass fraction (%))	76.7	70.5	73.6	55.2	52.9		73.6	4.22	54.0	3.06	80.5	3.3	71.9	1.27	-0.3	-0.9	0.28

^aCertified values are in bold^bSee text for explanation

Category	Number by Category		
	z (25%)	z (s)	p (15%)
	≤ 2	2 to 3	≥ 3
	10	13	17
	2	3	0
	5	1	0
	z (25%)	z (s)	p (15%)

PCB CONGENER ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)									Material Reference Values (ng/g wet mass)				Performance Scores ^a			
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		z-score	Homog VII	z-score
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	Uncert	(25%)	(s)	(15%)
18							3.45	3.30			3.4	3.1	6.57	12.6	4.35	0.56	
28	22.9	21.7	23.4	14.0	14.5	15.9	22.7	3.9	14.8	6.7	18.6	2.4	13.06	1.07	0.9	1.1	0.26
31	w/28	w/28	w/28	w/28	w/28	w/28	w/28		w/28		1.76	0.7	3.56	0.36			
44	47.4	43.5	47.7	13.3	11.4	15.9	46.2	5.1	13.5	16.7	46.2	3.1	12.1	0.51	0.0	0.0	0.34
49	86.2	80.7	88.1	18.2	17.6	18.7	85.0	4.5	18.2	3.0	88.7	7.0	18.3	0.04	-0.2	-0.4	0.30
52	280	258	276	35.3	38.9	40.6	271	4.3	38.3	7.1	271	20	40.7	1.30	0.0	0.0	0.29
66/95*	below	below	below	below	below	below	below		below								
87	204.0	185.0	196.0	21.4	22.9	24.0	195.0	4.9	22.8	5.7	201	18	20.6	2.55	-0.1	-0.3	0.33
99	480	434	483	55.8	58.6	61.9	466	5.9	58.8	5.2	465	40	58.5	5.17	0.0	0.0	0.39
101 (+90)	665	619	674	77.1	77.6	81.8	653	4.5	78.8	3.3	649	129	78.2	12.4	0.0	0.0	0.30
105	88.2	79.4	85.0	23.6	26.8	23.6	84.2	5.3	24.7	7.5	90	16	28.6	1.16	-0.3	-0.2	0.35
118	890	852	893	97.7	104	107	878	2.6	103	4.6	640	51	76.5	2.87	1.5	2.9	0.17
128				22.4	22.8	22.9			22.7	1.2	150	8.6	23.0	1.06			
132	w/153	w/153	w/153	w/153	w/153	w/153	w/153		w/153				21.1	4.75			
138 (+163+164)	1290	1200	1330	127	131	154	1273	5.2	137	10.6	1377	136	146	12.9	-0.3	-0.5	0.35
149	622	575	619	67.3	70.5	72.5	605	4.3	70	3.7	741	47	89.0	6.94	-0.7	-1.7	0.29
151	215	202	213	18.8	20.4	24.0	210	3.3	21.1	12.6	261	20	28.6	1.33	-0.8	-1.6	0.22
153	1960	1810	1950	213	226	233	1907	4.4	224	4.5	1831	240	228	9.75	0.2	0.2	0.29
156	87.0	84.6	95.1	10.4	11.1	11.4	88.9	6.2	10.9	4.8	98.2	15	11.4	0.95	-0.4	-0.4	0.41
170 (+190)	309	290	318	40.6	46.7	45.1	306	4.7	44.1	7.2	296	16	42.6	2.18	0.1	0.4	0.31
180	932	849	963	149	154	168	915	6.4	157	6.3	862	75	138	9.70	0.2	0.4	0.43
183	253	235	259	41.5	44.1	41.3	249	5.0	42.3	3.7	234	13	38.0	1.83	0.3	0.7	0.33
187	712	657	729	ND	112	119	699	5.4	116	4.3	710	72	121	11.1	-0.1	-0.1	0.36
194	112	102	116	48.8	50.4	51.8	110	6.6	50.3	3.0	127	15	53.5	5.18	-0.5	-0.8	0.44
195	31.5	inf	30.2	12.3	12.3	12.9	30.9	3.0	12.5	2.8	36.8	14	14.3	2.17	-0.6	-0.3	0.20
201	41.2	39.3	41.8	12.4	13.6	13.4	40.8	3.2	13.1	4.9	46.2	4.1	16.8	1.30	-0.5	-1.3	0.21
206	67.2	64.5	73.2	41.3	44.1	46.6	68.3	6.5	44.0	6.0	81.7	13	44.9	4.23	-0.7	-0.7	0.43
209	22.7	20.5	23.4	17.3	19.1	20.7	22.2	6.8	19.0	8.9	26.0	5.7	17.2	1.86	-0.6	-0.5	0.45
66	70.5	64.2	70.8	20.9	21.8	22.8	68.5	5.4	21.8	4.4	77.2	40	22.4	0.51	-0.4	-0.1	0.36
95				33.1	34.6	37.3			35.0	6.1	308	31	33.9	0.51			

^aCertified values are in bold ^bSee text for explanation

Category	Number by Category		
	z (25%)	z (s)	p (15%)
	≤ 2	2 to 3	≥ 3
	24	23	24
	0	1	0
	0	0	0

2005 EXERCISE FOR ORGANOCHLORINES IN MARINE MAMMAL TISSUES

Laboratory Number:

9

SAMPLES: Homogenate VII AND SRM 1945

PESTICIDE, PBDE, AND LIPID ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)										Material Reference Values (ng/g wet mass)				Performance Scores ^a		
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		Homog VII	SRM 1945	Performance Scores ^a
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	Uncert	z-score (25%)	z-score (s)	p-score (15%)
2,4'-DDT											428	243	90.9	13.5			
4,4'-DDT	2614	2089	1526	208	210	230	2076	26.2	216	5.6	2343	349	233	8.02	-0.5	-0.5	1.75
2,4'-DDE											78.4	9.3	14.2	1.39			
4,4'-DDE	7664	6612	6632	428	466	462	6969	8.6	452	4.6	7056	981	497	19.5	0.0	-0.1	0.58
2,4'-DDD											96.6	28	19.5	1.18			
4,4'-DDD	1300	1405	1040	100	104	84	1248	15.1	96	11.0	1286	255	120	4.87	-0.1	-0.1	1.00
HCB	236	185	195	29.0	26.0	25.0	205	13.2	27	7.8	267	23	30.6	1.45	-0.9	-1.7	0.88
α -HCH	<11	<15	<20	<17	<20	<44	<		<		4.12	1.2	16.9	1.41			
β -HCH																	
γ -HCH	<10	<13	<18	<22	<18	<44	<		<		2.12	2.5	3.18	0.01			
Heptachlor Epoxide											49.2	18	10.7	0.09			
Cis-Chlordane											49.4	18	48.1	1.58			
Trans-Chlordane											7.79	6.9	11.8	0.54			
Oxychlordane											258	33	21.2	1.06			
Cis-Nonachlor											232	12	45.8	3.29			
Trans-Nonachlor											1494	150	198	15.5			
Dieldrin	224	50	27	49.0	18.0	<38	100	107.4	34	65.4	175	53	50.1	4.05	-1.7	-1.0	7.16
Mirex											177	24	31.0	3.35			
PBDE 47											132	17	39.6	0.18			
PBDE 99											22.2	2.8	18.9	2.32			
PBDE 100											39.7	6.1	10.3	1.13			
PBDE 153											14.2	1.6	8.34	0.55			
PBDE 154											36.7	7.5	13.3	1.73			
Lipid (mass fraction (%))	83.0	80.9	82.1	74.8	74.2	70.9	82.0	1.28	73.3	2.86	80.5	3.3	71.9	1.27	0.1	0.2	0.09

^aCertified values are in bold ^bSee text for explanation

Category	Number by Category		
	z (25%)	z (s)	p (15%)
	≤ 2	6	5
2 to 3	0	0	0
≥ 3	0	0	1
	z (25%)	z (s)	p (15%)

PCB CONGENER ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)									Material Reference Values (ng/g wet mass)				Performance Scores ^a				
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		Homog VII	z-score (s)		
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab ng/g wet	lab %RSD	lab ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	Uncert	p-score (15%)			
18	41.0	<9	23.00	<2	<16	<3	32.0	40			6.57	12.6	4.35	0.56	15.5	1.98	2.65	
28	22.0	19.0	17.0	<11	<21	<14	19.3	13.0			18.6	2.4	13.06	1.07	0.2	0.20	0.87	
31	<8	<15	<11	<8	<20	<11					1.76	0.7	3.56	0.36				
44	56.0	39.0	53.0	<9	<17	<12	49.3	18.4			46.2	3.1	12.1	0.51	0.3	0.75	1.23	
49	126	74.0	103	17.0	18.0	<20	101	25.8	17.5	4.0	88.7	7.0	18.3	0.04	0.6	1.29	1.72	
52	317	216	254	37.0	28.0	28.0	262	19.4	31.0	16.8	271	20	40.7	1.30	-0.1	-0.27	1.30	
66/95*	below	below	below	below	below	below	below		below									
87											201	18	20.6	2.55				
99											465	40	58.5	5.17				
101 (+90)	743	567	625	95.0	74.0	69.0	645	13.9	79.3	17.4	649	129	78.2	12.4	0.0	-0.02	0.93	
105	98.0	75.0	88.0	30.0	36.0	31.0	87.0	13.3	32.3	9.9	90	16	28.6	1.16	-0.1	-0.12	0.88	
118	668	556	605	91.0	76.0	72.0	610	9.2	79.7	12.6	640	51	76.5	2.87	-0.2	-0.37	0.61	
128	187	151	182	28.0	28.0	29.0	173	11.3	28.3	2.0	150	8.6	23.0	1.06	0.6	1.67	0.75	
132													21.1	4.75				
138 (+163+164)	1420	1281	1277	181	137	149	1326	6.1	156	14.6	1377	136	146	12.9	-0.1	-0.22	0.41	
149	706	589	613	91.0	73.0	78.0	636	9.7	81	11.5	741	47	89.0	6.94	-0.6	-1.32	0.65	
151	276	216	234	31.0	24.0	25.0	242	12.7	26.7	14.2	261	20	28.6	1.33	-0.3	-0.61	0.85	
153	1944	1711	1837	242	194	210	1831	6.4	215	11.4	1831	240	228	9.75	0.0	0.00	0.42	
156	107.0	77.0	94.0	12.0	20.0	<10	92.7	16.2	16.0	35.4	98.2	15	11.4	0.95	-0.2	-0.23	1.08	
170 (+190)	372	300	330	54.0	46.0	47.0	334	10.8	49.0	8.9	296	16	42.6	2.18	0.5	1.51	0.72	
180	955	849	867	179	143	159	890	6.4	160	11.2	862	75	138	9.70	0.1	0.22	0.42	
183	258	190	219	43.0	36.0	37.0	222	15.3	38.7	9.8	234	13	38.0	1.83	-0.2	-0.56	1.02	
187	833	698	710	142	109	120	747	10.0	124	13.6	710	72	121	11.1	0.2	0.32	0.67	
194	155	111	138	69.0	52.0	62.0	135	16.5	61.0	14.0	127	15	53.5	5.18	0.2	0.35	1.10	
195											36.8	14	14.3	2.17				
201											46.2	4.1	16.8	1.30				
206											81.7	13	44.9	4.23				
209											26.0	5.7	17.2	1.86				
66	97.0	71.0	141	29.0	26.0	25.0	103	34.4	26.7	7.8	77.2	40	22.4	0.51	1.3	0.43	2.29	
95											308	31	33.9	0.51				
															Number by Category			
															Category	z (25%)	z (s)	p (15%)
															≤ 2	19	20	18
															2 to 3	0	0	2
															≥ 3	1	0	0

^aCertified values are in bold ^bSee text for explanation

SAMPLES: Homogenate VII AND SRM 1945

PESTICIDE, PBDE, AND LIPID ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)										Material Reference Values (ng/g wet mass)				Performance Scores ^a		
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		Homog VII	Homog VII	
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	Uncert	z-score (25%)	z-score (s)	p-score (15%)
2,4'-DDT	2200	2100	2450	260.0	210	190	2250	8.0	220	16.4	428	243	90.9	13.5	17.0	6.0	0.53
4,4'-DDT	3960	3750	4360	410	470	440	4023	7.7	440	6.8	2343	349	233	8.02	2.9	3.1	0.51
2,4'-DDE	260	260	310.0	<100	<100	<100	277	10.4			78.4	9.3	14.2	1.39	10.1	14.8	0.70
4,4'-DDE	5450	5860	5210	430	410	380	5507	6.0	407	6.2	7056	981	497	19.5	-0.9	-0.9	0.40
2,4'-DDD	650	640	720	90.0	100	90.0	670	6.5	93	6.2	96.6	28	19.5	1.18	23.7	13.3	0.43
4,4'-DDD	1650	1520	1780	170	150	140	1650	7.9	153	10.0	1286	255	120	4.87	1.1	0.9	0.53
HCB	130	140	170	<50	<50	<50	147	14.2	<50		267	23	30.6	1.45	-1.8	-3.3	0.95
α -HCH	<50	<50	<50	<50	<50	<50	<50		<50		4.12	1.2	16.9	1.41			
β -HCH																	
γ -HCH	<50	<50	<50	<50	<50	<50	<50		<50		2.12	2.5	3.2	0.01			
Heptachlor Epoxide	<50	<50	<50	<50	<50	<50	<50		<50		49.2	18	10.7	0.09			
Cis-Chlordane											49.4	18	48.1	1.58			
Trans-Chlordane	1360	1380	1550	<50	160	130	1430	7.3	145	14.6	7.79	6.9	11.8	0.54	730.0	180.5	0.49
Oxychlordane											258	33	21.2	1.06			
Cis-Nonachlor											232	12	45.8	3.29			
Trans-Nonachlor											1494	150	198	15.5			
Dieldrin	570	590	690	100	110	100	617	10.4	103	5.6	175	53	50.1	4.05	10.1	6.1	0.70
Mirex	350	360	380	160	110	110	363	4.2	127	22.8	177	24	31.0	3.35	4.2	6.8	0.28
PBDE 47											132	17	39.6	0.18			
PBDE 99											22.2	2.8	18.9	2.32			
PBDE 100											39.7	6.1	10.3	1.13			
PBDE 153											14.2	1.6	8.3	0.55			
PBDE 154											36.7	7.5	13.3	1.73			
Lipid (mass fraction (%))	79.6			63.0	63.7		79.6		63.4	0.78	80.5	3.3	71.9	1.27	0.0	-0.1	0.00

^aCertified values are in bold^bSee text for explanation

Category	Number by Category		
	z (25%)	z (s)	p (15%)
	≤ 2	2 to 3	≥ 3
	4	3	11
	1	0	0
	6	8	0
	z (25%)	z (s)	p (15%)

SAMPLES: Homogenate VII AND SRM 1945

PESTICIDE, PBDE, AND LIPID ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)										Material Reference Values (ng/g wet mass)				Performance Scores ^a		
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		Homog VII	z-score (25%)	
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	Uncert	z-score (s)	p-score (15%)	
2,4'-DDT											428	243	90.9	13.5			
4,4'-DDT											2343	349	233	8.02			
2,4'-DDE											78.4	9.3	14.2	1.39			
4,4'-DDE											7056	981	497	19.5			
2,4'-DDD											96.6	28	19.5	1.18			
4,4'-DDD											1286	255	120	4.87			
HCB											267	23	30.6	1.45			
α -HCH											4.12	1.2	16.9	1.41			
β -HCH											2.12	2.5	3.18	0.01			
γ -HCH											49.2	18	10.7	0.09			
Heptachlor Epoxide											49.4	18	48.1	1.58			
Cis-Chlordane											7.79	6.9	11.8	0.54			
Trans-Chlordane											258	33	21.2	1.06			
Oxychlordane											232	12	45.8	3.29			
Cis-Nonachlor											1494	150	198	15.5			
Trans-Nonachlor											175	53	50.1	4.05			
Dieldrin											177	24	31.0	3.35			
Mirex																	
PBDE 47	117	121	120	36.0	35.0	NA	119	1.7	36	2.0	132	17	39.6	0.18	-0.4	-0.5	0.12
PBDE 99	21.0	21.9	22.1	16.8	16.1	NA	22	2.8	16	3.0	22.2	2.8	18.9	2.32	-0.1	-0.2	0.19
PBDE 100	38.7	42.9	42.6	10.9	9.8	NA	41	5.7	10	7.6	39.7	6.1	10.3	1.13	0.2	0.2	0.38
PBDE 153	12.3	13.4	13.6	8.3	8.4	NA	13	5.3	8	0.4	14.2	1.6	8.34	0.55	-0.3	-0.6	0.36
PBDE 154	35.1	35.9	36.6	12.3	12.4	NA	36	2.1	12	0.6	36.7	7.5	13.3	1.73	-0.1	-0.1	0.14
Lipid (mass fraction (%))	77.2	79.1	77.7	69.4	69.7	68.8	78.0	1.28	69.3	0.68	80.5	3.3	71.9	1.27	-0.1	-0.3	0.09

^aCertified values are in bold^bSee text for explanation

Category	Number by Category		
	z (25%)	z (s)	p (15%)
	≤ 2	6	6
	2 to 3	0	0
≥ 3		0	0
		z (25%)	z (s)
		0	0
		p (15%)	0

SAMPLES: Homogenate VII AND SRM 1945

PESTICIDE, PBDE, AND LIPID ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)										Material Reference Values (ng/g wet mass)				Performance Scores ^a		
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		Homog VII	z-score (25%)	
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	Uncert	z-score (s)	z-score (s)	p-score (15%)
2,4'-DDT	1583	1577	1559	167.6	174	191	1573	0.8	178	6.7	428	243	90.9	13.5	10.7	3.8	0.05
4,4'-DDT	3831	4349	4267	352	368	394	4149	6.7	372	5.7	2343	349	233	8.02	3.1	3.4	0.45
2,4'-DDE											78.4	9.3	14.2	1.39			
4,4'-DDE	7420	7017	7060	473	514	544	7166	3.1	510	7.0	7056	981	497	19.5	0.1	0.1	0.21
2,4'-DDD	81.4	71.9	71.5	16.9	18.3	18.8	75	7.5	18.0	5.6	96.6	28	19.5	1.18	-0.9	-0.5	0.50
4,4'-DDD	1347	1371	1365	100	100	105	1361	0.9	102	2.7	1286	255	120	4.87	0.2	0.2	0.06
HCB	255	259	260	28.6	28.5	28.7	258	1.0	28.6	0.4	267	23	30.6	1.45	-0.1	-0.2	0.07
α -HCH	3.75	3.55	3.66	13.9	13.8	14.1	3.66	2.9	13.9	0.9	4.12	1.2	16.9	1.41	-0.5	-0.4	0.19
β -HCH	5.56	5.73	6.07	2.06	1.86	1.95	5.79	4.5	1.96	4.9							
γ -HCH	0.92	0.84	0.84	2.46	2.45	2.58	0.87	5.1	2.50	3.0	2.12	2.5	3.18	0.01	-2.4	-0.7	0.34
Heptachlor Epoxide											49.2	18	10.7	0.09			
Cis-Chlordane	62.9	61.4	61.1	51.2	51.4	53.6	61.8	1.5	52.0	2.6	49.4	18	48.1	1.58	1.0	0.5	0.10
Trans-Chlordane	21.72	24.26	24.65	15.0	14.8	15.4	23.5	6.8	15.1	2.1	7.79	6.9	11.8	0.54	8.1	2.0	0.45
Oxychlordane	292	268	265	20.0	21.1	21.2	275	5.4	20.7	3.3	258	33	21.2	1.06	0.3	0.3	0.36
Cis-Nonachlor	699	675	643	106	115	122	672	4.1	115	7.3	232	12	45.8	3.29	7.6	26.6	0.28
Trans-Nonachlor	1732	1767	1712	185	188	195	1737	1.6	189	2.8	1494	150	198	15.5	0.6	1.1	0.11
Dieldrin											175	53	50.1	4.05			
Mirex	231	236	235	46.9	44.0	43.1	234	1.2	44.7	4.4	177	24	31.0	3.35	1.3	2.1	0.08
PBDE 47	114	93	102	39.0	36.4	38.0	103	10.3	37.8	3.4	132	17	39.6	0.18	-0.9	-1.2	0.69
PBDE 99	23.8	16.1	17.9	15.5	18.4	15.5	19.2	20.9	16.5	10.2	22.2	2.8	18.9	2.32	-0.5	-0.9	1.39
PBDE 100	27.9	23.6	25.4	9.73	8.84	9.14	25.6	8.4	9.24	4.9	39.7	6.1	10.3	1.13	-1.4	-1.7	0.56
PBDE 153	13.7	11.0	13.0	8.21	8.42	8.52	12.6	10.8	8.38	1.9	14.2	1.6	8.34	0.55	-0.5	-0.8	0.72
PBDE 154	30.0	25.7	28.4	13.1	12.5	13.3	28.0	7.7	13.0	3.1	36.7	7.5	13.3	1.73	-0.9	-0.9	0.51
Lipid (mass fraction (%))	88.3	89.9	89.6	77.3	76.1	76.2	89.3	0.97	76.5	0.85	80.5	3.3	71.9	1.27	0.4	1.2	0.06

^aCertified values are in bold^bSee text for explanation

Category	Number by Category		
	z (25%)	z (s)	p (15%)
	≤ 2	15	16
2 to 3			0
≥ 3	4	3	0
	z (25%)	z (s)	p (15%)

PCB CONGENER ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)									Material Reference Values (ng/g wet mass)				Performance Scores ^a			
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		z-score	Homog VII	z-score
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	Uncert	(25%)	(s)	(15%)
18																	
28	20.7	19.5	19.9	10.3	10.3	10.8	20.0	3.2	10.5	3.0	18.6	2.4	13.06	1.07	0.3	0.39	0.21
31	17.5	15.6	16.1	6.92	7.86	8.32	16.4	6.0	7.70	9.3	1.76	0.7	3.56	0.36	33.3	22.25	0.40
44																	
49																	
52	258	259	260	36.7	38.4	40.1	259	0.4	38.4	4.5	271	20	40.7	1.30	-0.2	-0.36	0.03
66/95*	below	below	below	below	below	below	below										
87																	
99	483	490	475	66.9	66.3	68.6	483	1.5	67.3	1.8	465	40	58.5	5.17	0.1	0.26	0.10
101 (+90)	575	590	572	80.5	81.0	82.3	579	1.6	81.3	1.1	649	129	78.2	12.4	-0.4	-0.38	0.11
105	103.2	106.3	105.2	31.4	31.4	31.8	104.9	1.5	31.5	0.8	90	16	28.6	1.16	0.6	0.54	0.10
118	578	594	577	80.5	78.4	85.5	583	1.7	81.5	4.5	640	51	76.5	2.87	-0.4	-0.70	0.11
128	163	148	145	22.2	23.5	24.2	152	6.4	23.3	4.3	150	8.6	23.0	1.06	0.1	0.14	0.43
132																	
138 (+163+164)	1527	1543	1450	164	163	182	1507	3.3	170	6.2	1377	136	146	12.9	0.4	0.57	0.22
149	644	663	651	67.1	69.4	72.2	653	1.5	69.6	3.6	741	47	89.0	6.94	-0.5	-1.11	0.10
151	286	300	295	35.0	31.2	31.4	294	2.4	32.5	6.7	261	20	28.6	1.33	0.5	1.00	0.16
153	1948	2026	1959	237	245	252	1977	2.1	245	3.0	1831	240	228	9.75	0.3	0.45	0.14
156	111	116	109	12.4	13.5	14.1	112	3.4	13.4	6.4	98.2	15	11.4	0.95	0.6	0.57	0.23
170 (+190)	292	318	303	42.4	45.0	45.6	305	4.3	44.3	3.8	296	16	42.6	2.18	0.1	0.35	0.28
180	971	1064	1034	155	150	156	1023	4.7	153	2.2	862	75	138	9.70	0.7	1.21	0.31
183	189	210	198	36.4	37.4	39.2	199	5.3	37.7	3.9	234	13	38.0	1.83	-0.6	-1.67	0.35
187	475	489	469	81.3	84.1	86.4	478	2.1	83.9	3.0	710	72	121	11.1	-1.3	-1.99	0.14
194	149	160	138	57.0	58.8	65.3	149	7.6	60.3	7.2	127	15	53.5	5.18	0.7	1.01	0.50
195																	
201																	
206	95.8	91.1	90.2	50.5	52.8	55.3	92.4	3.3	52.9	4.5	81.7	13	44.9	4.23	0.5	0.55	0.22
209	37.9	35.9	36.8	18.6	20.3	20.5	36.9	2.8	19.8	5.4	26.0	5.7	17.2	1.86	1.7	1.32	0.19
66	242.9	251.1	242.7	25.5	24.8	25.7	245.6	2.0	25.4	1.8	77.2	40	22.4	0.51	8.7	2.78	0.13
95																	

^aCertified values are in bold ^bSee text for explanation

Category	Number by Category		
	z (25%)	z (s)	p (15%)
	≤ 2	2 to 3	≥ 3
	19	19	21
	0	1	0
	2	1	0

SAMPLES: Homogenate VII AND SRM 1945

PESTICIDE, PBDE, AND LIPID ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)								Material Reference Values (ng/g wet mass)				Performance Scores ^a		
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		Homog VII
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	Uncert	z-score (25%)
2,4'-DDT											428	243	90.9	13.5	
4,4'-DDT											2343	349	233	8.02	
2,4'-DDE											78.4	9.3	14.2	1.39	
4,4'-DDE											7056	981	497	19.5	
2,4'-DDD											96.6	28	19.5	1.18	
4,4'-DDD											1286	255	120	4.87	
HCB											267	23	30.6	1.45	
α -HCH											4.12	1.2	16.9	1.41	
β -HCH											2.12	2.5	3.18	0.01	
γ -HCH											49.2	18	10.7	0.09	
Heptachlor Epoxide											49.4	18	48.1	1.58	
Cis-Chlordane											7.79	6.9	11.8	0.54	
Trans-Chlordane											258	33	21.2	1.06	
Oxychlordane											232	12	45.8	3.29	
Cis-Nonachlor											1494	150	198	15.5	
Trans-Nonachlor											175	53	50.1	4.05	
Dieldrin											177	24	31.0	3.35	
Mirex															
PBDE 47	123		119	35.8	36.7	36.7	121	2.6	36.4	1.4	132	17	39.6	0.18	-0.3
PBDE 99	23.6	22.0	21.1	16.5	16.0	16.8	22.2	5.7	16.4	2.5	22.2	2.8	18.9	2.32	0.0
PBDE 100	35.9	34.7	33.3	9.20	9.10	9.00	34.6	3.8	9.10	1.1	39.7	6.1	10.3	1.13	-0.5
PBDE 153	13.0	12.2	12.5	7.90	7.00	7.60	12.6	3.2	7.50	6.1	14.2	1.6	8.34	0.55	-0.5
PBDE 154	34.6	32.4	33.1	11.1	10.5	11.1	33.4	3.4	10.9	3.2	36.7	7.5	13.3	1.73	-0.4
Lipid (mass fraction (%))	87.9	87.8	83.0	72.9	76.0	76.6	86.2	3.25	75.2	2.64	80.5	3.3	71.9	1.27	0.3

^aCertified values are in bold^bSee text for explanation

Category	Number by Category		
	z (25%)	z (s)	p (15%)
	≤ 2	6	6
	2 to 3	0	0
≥ 3	0	0	0
		z (25%)	z (s)
		p (15%)	

PCB CONGENER ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)									Material Reference Values (ng/g wet mass)				Performance Scores ^a			
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		z-score	Homog VII	z-score
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	Uncert	(25%)	(s)	(15%)
18																	
28	26.4	24.8	23.8	12.8	12.7	11.7	25.0	5.2	12.4	4.9	18.6	2.4	13.06	1.07	1.4	1.8	0.3
31	< 2	< 2	< 2	3.0	1.7	2.1	<2		2.27	29	1.76	0.7	3.56	0.36			
44											46.2	3.1	12.1	0.51			
49											88.7	7.0	18.3	0.04			
52	355	346	332	44.0	44.8	42.8	344	3.3	43.9	2.3	271	20	40.7	1.30	1.1	2.2	0.2
66/95*	below	below	below	below	below	below	below				201	18	20.6	2.55			
87											465	40	58.5	5.17	-1.2	-2.1	0.2
99	312	335	327	43.6	44.3	44.1	324	3.6	44.0	0.8	649	129	78.2	12.4	-1.1	-1.0	0.2
101 (+90)	447	481	467	61.7	62.7	62.6	465	3.6	62.3	0.9	90	16	28.6	1.16	0.1	0.0	0.1
105	90.0	93.8	91.1	29.4	29.1	29.9	91.6	2.1	29.5	1.4	640	51	76.5	2.87	-0.5	-1.1	0.1
118	543	564	553	73.9	74.6	75.1	553	1.9	74.5	0.8	150	8.6	23.0	1.06	-0.2	-0.4	0.2
128	140	148	145	22.7	24.1	23.3	144	3.0	23.4	3.0			21.1	4.75			
132											1377	136	146	12.9	-0.9	-1.4	0.2
138 (+163+164)	1038	1088	1061	132	134	135	1062	2.4	133	1.3	741	47	89.0	6.94	0.3	0.6	0.2
149	768	817	794	94.8	95.7	96.5	793	3.1	96	0.9			261	20	28.6	1.33	
151											1831	240	228	9.75	-0.3	-0.4	0.2
153	1667	1746	1697	208	212	213	1703	2.3	211	1.1	296	16	42.6	2.18	-0.5	-1.5	0.3
156	75.8	76.4	77.6	9.90	10.0	10.7	76.6	1.2	10.2	4.3	862	75	138	9.70	-1.5	-2.4	0.2
170 (+190)	246	267	259	38.3	39.6	39.4	257	4.0	39.1	1.8	710	72	121	11.1	-0.8	-1.2	0.2
180	523	557	540	98.1	101	100	540	3.1	100	1.3	127	15	53.5	5.18	-1.6	-2.3	0.2
183	199	212	207	36.0	37.0	36.7	206	3.0	36.6	1.4	36.8	14	14.3	2.17			
187	554	588	574	101	104	104	572	3.0	103	1.5	46.2	4.1	16.8	1.30			
194	74.0	79.7	77.1	37.0	38.1	38.0	76.9	3.7	37.7	1.6	81.7	13	44.9	4.23			
195											26.0	5.7	17.2	1.86			
201											77.2	40	22.4	0.51			
206																	
209																	
66																	
95	242	265	257	33.3	32.9	32.9	255	4.5	33.0	0.7	308	31	33.9	0.51	-0.7	-1.4	0.3

^aCertified values are in bold ^bSee text for explanation

Category	Number by Category		
	z (25%)	z (s)	p (15%)
≤ 2	17	13	17
2 to 3	0	4	0
≥ 3	0	0	0

SAMPLES: Homogenate VII AND SRM 1945

PESTICIDE, PBDE, AND LIPID ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)										Material Reference Values (ng/g wet mass)				Performance Scores ^a		
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		Homog VII	Homog VII	Homog VII
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	Uncert	z-score (25%)	z-score (s)	p-score (15%)
2,4'-DDT											428	243	90.9	13.5			
4,4'-DDT	1332	956	1048	476	298	376	1112	17.6	383	23.3	2343	349	233	8.02	-2.1	-2.3	1.18
2,4'-DDE											78.4	9.3	14.2	1.39			
4,4'-DDE	2982	2213	2418	361	350	354	2538	15.7	355	1.7	7056	981	497	19.5	-2.6	-2.6	1.05
2,4'-DDD											96.6	28	19.5	1.18			
4,4'-DDD	637	828	814	74.4	79.3	81.0	760	14.0	78.2	4.4	1286	255	120	4.87	-1.6	-1.3	0.93
HCB											267	23	30.6	1.45			
α -HCH	<5ppb	<5ppb	<5ppb	7.90	7.30	6.70			7.30	8.2	4.12	1.2	16.9	1.41			
β -HCH	10.2	5.10	5.80	5.60	5.40	4.10	7.03	39.3	5.03	16.2							
γ -HCH	<5ppb	<5ppb	<5ppb	<5ppb	<5ppb	<5ppb	<5ppb				2.12	2.5	3.18	0.01			
Heptachlor Epoxide	18.8	13.8	16.3	10.0	9.60	9.10	16.3	15.3	9.57	4.7	49.2	18	10.7	0.09	-2.7	-1.8	1.02
Cis-Chlordane	125.9	64.4	70.3	24.2	24.8	25.5	86.9	39.1	24.8	2.6	49.4	18	48.1	1.58	3.0	1.4	2.60
Trans-Chlordane											7.79	6.9	11.8	0.54			
Oxychlordane	117	169	180	21.1	22.5	19.9	155	21.6	21.2	6.1	258	33	21.2	1.06	-1.6	-2.0	1.44
Cis-Nonachlor											232	12	45.8	3.29			
Trans-Nonachlor											1494	150	198	15.5			
Dieldrin	110	55.4	59.6	57.2	49.3	49.5	75.0	40.5	52.0	8.7	175	53	50.1	4.05	-2.3	-1.4	2.70
Mirex											177	24	31.0	3.35			
PBDE 47											132	17	39.6	0.18			
PBDE 99											22.2	2.8	18.9	2.32			
PBDE 100											39.7	6.1	10.3	1.13			
PBDE 153											14.2	1.6	8.34	0.55			
PBDE 154											36.7	7.5	13.3	1.73			
Lipid (mass fraction (%))	78.2	76.9	77.2	67.1	63.1	64.5	77.4	0.88	64.9	3.13	80.5	3.3	71.9	1.27	-0.2	-0.4	0.06

^aCertified values are in bold ^bSee text for explanation

Category	Number by Category		
	z (25%)	z (s)	p (15%)
	≤ 2	2 to 3	≥ 3
	3	6	6
	4	2	2
	1	0	0
	z (25%)	z (s)	p (15%)

SAMPLES: Homogenate VII AND SRM 1945

PESTICIDE, PBDE, AND LIPID ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)										Material Reference Values (ng/g wet mass)				Performance Scores ^a		
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		Homog VII	Homog VII	
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	Uncert	z-score (25%)	z-score (s)	p-score (15%)
2,4'-DDT	300	323	328	67.0	74.0	72.0	317	4.7	71.0	5.1	428	243	90.9	13.5	-1.0	-0.4	0.31
4,4'-DDT	1520	1560	1580	190	177	174	1553	2.0	180	4.7	2343	349	233	8.02	-1.3	-1.5	0.13
2,4'-DDE	51.0	61.0	62.0	21.0	16.0	15.0	58.0	10.5	17.3	18.5	78.4	9.3	14.2	1.39	-1.0	-1.5	0.70
4,4'-DDE	5560	5840	5710	428	426	382	5703	2.5	412	6.3	7056	981	497	19.5	-0.8	-0.8	0.16
2,4'-DDD	59.0	42.0	42.0	15.0	26.0	18.0	47.7	20.6	19.7	28.9	96.6	28	19.5	1.18	-2.0	-1.1	1.37
4,4'-DDD	965	990	995	102	104	111	983	1.6	106	4.5	1286	255	120	4.87	-0.9	-0.7	0.11
HCB	204	224	195	24.7	25.6	27.5	208	7.1	25.9	5.5	267	23	30.6	1.45	-0.9	-1.6	0.48
α -HCH	3.60	3.10	3.80	13.0	13.0	13.0	3.50	10	13.0	0.0	4.12	1.2	16.9	1.41	-0.6	-0.5	0.69
β -HCH	<2	<2	<2	7.50	4.30	7.20	<2		6.33	27.9							
γ -HCH	2.90	3.00	4.20	3.70	3.40	3.00	3.37	21.5	3.37	10.4	2.12	2.5	3.18	0.01	2.4	0.7	1.43
Heptachlor Epoxide	75.0	65.0	69.0	17.0	16.0	16.0	69.7	7.2	16.3	3.5	49.2	18	10.7	0.09	1.7	1.1	0.48
Cis-Chlordane	46.0	52.0	55.0	43.0	37.0	45.0	51.0	9.0	41.7	10.0	49.4	18	48.1	1.58	0.1	0.1	0.60
Trans-Chlordane	<2	<2	<2	13.0	13.0	12.0	<2		12.7	4.6	7.79	6.9	11.8	0.54			
Oxychlordane	244	231	236	18.0	18.0	16.0	237	2.8	17.3	6.7	258	33	21.2	1.06	-0.3	-0.4	0.18
Cis-Nonachlor	235	221	226	54.0	58.0	46.0	227	3.1	52.7	11.6	232	12	45.8	3.29	-0.1	-0.3	0.21
Trans-Nonachlor	1430	1310	1320	156	152	151	1353	4.9	153	1.7	1494	150	198	15.5	-0.4	-0.6	0.33
Dieldrin	137	108	138	42.0	40.0	42.0	128	13.3	41.3	2.8	175	53	50.1	4.05	-1.1	-0.7	0.89
Mirex	165	147	154	14.0	20.0	22.0	155	5.8	18.7	22.3	177	24	31.0	3.35	-0.5	-0.8	0.39
PBDE 47	87.4	143	136	32.8	33.2	30.8	122	24.8	32.3	4.0	132	17	39.6	0.18	-0.3	-0.4	1.65
PBDE 99	60.0	85.1	83.0	43.0	47.1	50.5	76.0	18.3	46.9	8.0	22.2	2.8	18.9	2.32	9.7	16.9	1.22
PBDE 100	24.3	31.7	30.7	9.05	9.58	9.55	28.9	13.9	9.39	3.2	39.7	6.1	10.3	1.13	-1.1	-1.3	0.93
PBDE 153	27.3	37.1	41.4	10.2	12.3	15.2	35.3	20.5	12.6	20.0	14.2	1.6	8.34	0.55	5.9	10.6	1.37
PBDE 154	13.4	20.0	19.3	5.79	7.80	11.2	17.6	20.6	8.26	33.1	36.7	7.5	13.3	1.73	-2.1	-2.0	1.38
Lipid (mass fraction (%))	84.9	84.2	85.2	74.7	71.3	71.0	84.8	0.61	72.3	2.84	80.5	3.3	71.9	1.27	0.2	0.6	0.04

^aCertified values are in bold^bSee text for explanation

PCB CONGENER ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)									Material Reference Values (ng/g wet mass)					Performance Scores ^a		
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		z-score	Homog VII	z-score
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	Uncert	(25%)	(s)	(15%)
18	3.45	4.81	4.48	2.66	2.83	2.21	4.25	17	2.57	12.5	6.57	12.6	4.35	0.56	-1.4	-0.18	1.11
28	14.3	15.1	13.8	13.4	9.19	11.9	14.4	4.6	11.5	18.6	18.6	2.4	13.06	1.07	-0.9	-1.17	0.30
31	0.580	0.350	0.320	4.33	4.57	4.24	0.4	34.1	4.38	3.9	1.76	0.7	3.56	0.36	-3.1	-2.04	2.28
44	36.5	47.2	48.7	9.63	11.6	11.6	44.1	15.1	10.9	10.4	46.2	3.1	12.1	0.51	-0.2	-0.49	1.00
49	73.0	64.2	71.6	17.5	17.0	16.2	69.6	6.8	16.9	3.9	88.7	7.0	18.3	0.04	-0.9	-2.01	0.45
52	268	309	270	33.3	32.5	37.3	282	8.2	34.4	7.5	271	20	40.7	1.30	0.2	0.33	0.55
66/95*	Below	Below	Below	Below	Below	Below	Below										
87																	
99	315	348	393	60.1	60.4	55.4	352	11.1	58.6	4.8	465	40	58.5	5.17	-1.0	-1.67	0.74
101 (+90)	1190	1170	850	82.7	71.0	84.4	1070	17.8	79.4	9.2	649	129	78.2	12.4	2.6	2.27	1.19
105	164	192	175	26.8	25.3	23.9	177	8.0	25.3	5.7	90.3	16	28.6	1.16	3.8	3.17	0.53
118	592	691	652	63.1	66.5	71.6	645	7.7	67.1	6.4	640	51	76.5	2.87	0.0	0.06	0.52
128	164	179	171	23.6	26.4	29.6	171	4.4	26.5	11.3	150	8.6	23.0	1.06	0.6	1.52	0.29
132	159.0	127.0	96.0	33.3	34.9	38.1	127	24.7	35.4	6.9			21.1	4.75			
138 (+163+164)	1450	1810	1750	159	184	176	1670	11.5	173	7.4	1377	136	146	12.9	0.9	1.28	0.77
149	665	839	657	68.6	72.1	81.5	720	14.3	74.1	9.0	741	47	89.0	6.94	-0.1	-0.26	0.95
151	246	267	248	23.5	25.7	29.4	254	4.6	26.2	11.4	261	20	28.6	1.33	-0.1	-0.24	0.30
153	1300	1330	1330	188	184	172	1320	1.3	181	4.6	1831	240	228	9.75	-1.1	-1.57	0.09
156	151	171	143	12.8	12.8	12.1	155	9.3	12.6	3.2	98.2	15	11.4	0.95	2.3	2.40	0.62
170 (+190)	241	262	241	30.7	32.9	35.3	248	4.9	33.0	7.0	296	16	42.6	2.18	-0.6	-1.89	0.33
180	578	662	609	111	109	100	616	6.9	107	5.5	862	75	138	9.70	-1.1	-1.85	0.46
183	228	260	238	31.1	31.2	29.2	242	6.8	30.5	3.7	234	13	38.0	1.83	0.1	0.36	0.45
187	575	644	608	93.6	95.3	102	609	5.7	97.0	4.6	710	72	121	11.1	-0.6	-0.86	0.38
194	149	176	160	30.5	32.4	33.2	162	8.4	32.0	4.3	127	15	53.5	5.18	1.1	1.59	0.56
195	79.7	83.2	88.3	14.4	15.0	16.5	83.7	5.2	15.3	7.1	36.8	14	14.3	2.17	5.1	2.25	0.34
201	268	310	297	46.4	69.5	45.1	292	7.4	53.7	25.6	46.2	4.1	16.8	1.30	21.3	58.85	0.49
206	106	153	134	33.2	36.6	38.0	131	18.0	35.9	6.9	81.7	13	44.9	4.23	2.4	2.55	1.20
209	48.9	39.8	38.9	13.5	14.9	15.4	42.5	13.0	14.6	6.7	26.0	5.7	17.2	1.86	2.6	2.00	0.87
66	110	110	100	25.7	23.2	17.7	106.7	5.4	22.2	18.4	77.2	40	22.4	0.51	1.5	0.49	0.36
95	309	348	321	36.4	38.1	44.9	326	6.1	39.8	11.3	308	31	33.9	0.51	0.2	0.46	0.41

^aCertified values are in bold ^bSee text for explanation

Category	Number by Category		
	z (25%)	z (s)	p (15%)
	≤ 2	2 to 3	≥ 3
	19	18	26
	4	7	1
	4	2	0

SAMPLES: Homogenate VII AND SRM 1945

PESTICIDE, PBDE, AND LIPID ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)								Material Reference Values (ng/g wet mass)				Performance Scores ^a				
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		Homog VII		
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	Uncert	z-score (25%)	z-score (s)	p-score (15%)
2,4'-DDT	350	375		<20	<20		363	4.9	<20		428	243	90.9	13.5	-0.6	-0.2	0.33
4,4'-DDT	3090	3620		236	261		3355	11.2	249	7.1	2343	349	233	8.02	1.7	1.9	0.74
2,4'-DDE	<20	<20		<20	<20		<20		<20		78.4	9.3	14.2	1.39			
4,4'-DDE	8870	8570		430	478		8720	2.4	454	7.5	7056	981	497	19.5	0.9	1.0	0.16
2,4'-DDD	<20	<20		<20	<20		<20		<20		96.6	28	19.5	1.18			
4,4'-DDD	1870	2010		151	168		1940	5.1	160	7.5	1286	255	120	4.87	2.0	1.6	0.34
HCB											267	23	30.6	1.45			
α -HCH	<20	<20		<20	<20		<20		<20		4.12	1.2	16.9	1.41			
β -HCH	<20	<20		<20	<20		<20		<20								
γ -HCH	<20	<20		<20	<20		<20		<20		2.12	2.5	3.18	0.01			
Heptachlor Epoxide	<20	<20		<20	<20		<20		<20		49.2	18	10.7	0.09			
Cis-Chlordane	<20	<20		<20	<20		<20		<20		49.4	18	48.1	1.58			
Trans-Chlordane	<20	<20		<20	<20		<20		<20		7.79	6.9	11.8	0.54			
Oxychlordane	155	159		<20	<20		157	1.8	<20		258	33	21.2	1.06	-1.6	-1.9	0.12
Cis-Nonachlor	198	220		44.0	48.0		209	7.4	46	6.1	232	12	45.8	3.29	-0.4	-1.4	0.50
Trans-Nonachlor	108	124		91.0	96.0		116	9.8	94	3.8	1494	150	198	15.5	-3.7	-6.0	0.65
Dieldrin	417	422		82.0	81.0		420	0.8	82	0.9	175	53	50.1	4.05	5.6	3.4	0.06
Mirex	<20	<20		<20	<20		<20		<20		177	24	31.0	3.35			
PBDE 47											132	17	39.6	0.18			
PBDE 99											22.2	2.8	18.9	2.32			
PBDE 100											39.7	6.1	10.3	1.13			
PBDE 153											14.2	1.6	8.34	0.55			
PBDE 154											36.7	7.5	13.3	1.73			
Lipid (mass fraction (%))											80.5	3.3	71.9	1.27			

^aCertified values are in bold^bSee text for explanation

Category	Number by Category		
	z (25%)	z (s)	p (15%)
	≤ 2	2 to 3	≥ 3
	5	6	8
	1	0	0
	2	2	0
	z (25%)	z (s)	p (15%)

SAMPLES: Homogenate VII AND SRM 1945

PESTICIDE, PBDE, AND LIPID ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)										Material Reference Values (ng/g wet mass)				Performance Scores ^a		
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		Homog VII	z-score (25%)	
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	Uncert	z-score (s)	z-score (s)	p-score (15%)
2,4'-DDT	2848	2244	385	279	207	313	1826	70.3	266	20.4	428	243	90.9	13.5	13.1	4.6	4.7
4,4'-DDT	7876	6274	914	398	269	443	5021	72.6	370	24.4	2343	349	233	8.02	4.6	5.0	4.8
2,4'-DDE											78.4	9.3	14.2	1.39			
4,4'-DDE	2322	690	152	68.3	72.1	117	1055	107	86	31.5	7056	981	497	19.5	-3.4	-3.5	7.1
2,4'-DDD											96.6	28	19.5	1.18			
4,4'-DDD	561	2814	482	177	119	204	1286	103	167	26.1	1286	255	120	4.87	0.0	0.0	6.9
HCB	189	322	31.2	42.7	39.5	38.6	181	80.6	40	5.5	267	23	30.6	1.45	-1.3	-2.3	5.4
a-HCH				22.1	15.1	23.8			20	22.6	4.12	1.2	16.9	1.41			
b-HCH																	
g-HCH				4.1	2.8	4.6			4	24.6	2.12	2.5	3.2	0.01			
Heptachlor Epoxide	268			15.1	10.4	16.6	268		14	22.9	49.2	18	10.7	0.09	17.8	11.7	0.0
Cis-Chlordane	200	73.8	11.4	24.3	15.7	28.2	95	101	23	28.0	49.4	18	48.1	1.58	3.7	1.7	6.7
Trans-Chlordane	149	79.6	14.0	75.6	50.1	86.3	81	83.5	71	26.3	7.79	6.9	11.8	0.54	37.5	9.3	5.6
Oxychlordane											258	33	21.2	1.06			
Cis-Nonachlor											232	12	45.8	3.29			
Trans-Nonachlor											1494	150	198	15.5			
Dieldrin											175	53	50.1	4.05			
Mirex	321	224	24.7	54.1	53.4	58.8	190	79.5	55	5.3	177	24	31.0	3.35	0.3	0.5	5.3
PBDE 47											132	17	39.6	0.18			
PBDE 99											22.2	2.8	18.9	2.32			
PBDE 100											39.7	6.1	10.3	1.13			
PBDE 153											14.2	1.6	8.3	0.55			
PBDE 154											36.7	7.5	13.3	1.73			
Lipid (mass fraction (%))	86.4	87.3	85.0	73.0	77.5	74.6	86.2	1.37	75.0	3.05	80.5	3.3	71.9	1.27	0.3	0.8	0.1

^aCertified values are in bold^bSee text for explanation

PCB CONGENER ANALYSES Date(s) of measurements	Data as Submitted by Laboratory (ng/g wet mass)										Material Reference Values (ng/g wet mass)				Performance Scores ^a		
	Homog VII			SRM 1945			Homog VII		SRM 1945		Homog VII		SRM 1945		Homog VII	Homog VII	Homog VII
	Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD	Assigned Value	95% CL	Target ^b Value	95% CL	z-score (25%)	z-score (s)	p-score (15%)
18	11.9	7.07	1.55	9.84	9.30	5.35	6.84	76	8.16	30	6.57	12.6	4.35	0.56	0.2	0.02	5.04
28	5.28	10.2	1.43	5.62	5.94	5.49	5.65	78	5.68	4	18.6	2.4	13.06	1.07	-2.8	-3.60	5.20
31	0.949	1.28	0.17	2.89	3.20	2.91	0.799	72	3.00	6	1.76	0.7	3.56	0.36	-2.2	-1.46	4.77
44	5.92	11.8	1.34	3.79	4.05	4.30	6.34	82	4.05	6	46.2	3.1	12.1	0.51	-3.5	-9.52	5.50
49	27.5	45.3	4.5	11.4	10.9	10.3	25.8	79	10.8	5	88.7	7.0	18.3	0.04	-2.8	-6.62	5.29
52	45.2	113	10.8	19.0	18.9	17.5	56.4	92	18.5	5	271	20	40.7	1.30	-3.2	-6.39	6.16
66/95*																	
87	18.7	94.6	7.24	12.8	13.2	11.9	40.2	118	12.6	5	201	18	20.6	2.55	-3.2	-9.84	7.87
99	307	366	28.6	49.5	51.0	47.3	234	77	49.2	4	465	40	58.5	5.17	-2.0	-3.40	5.14
101 (+90)	162	347	25.2	46.8	43.4	41.4	178	91	43.8	6	649	129	78.2	12.4	-2.9	-2.54	6.04
105	1.61	24.5	2.36	10.3	11.5	10.7	9.5	137	10.8	6	90	16	28.6	1.16	-3.6	-2.95	9.14
118	77.2	351	23.8	44.5	42.4	40.8	151	116	42.6	4	640	51	76.5	2.87	-3.1	-5.99	7.77
128	69.2	141.1	12.4	22.6	22.8	22.9	74.2	87	22.8	1	150	8.6	23.0	1.06	-2.0	-5.50	5.79
132	16.1	64.6	7.68	8.91	9.75	9.48	29.5	104	9.38	5			21.1	4.75			6.95
138 (+163+164)	242	736	51.7	88.9	83.3	79.6	343	103	84.0	6	1377	136	146	12.9	-3.0	-4.50	6.86
149	194	336	24.6	41.5	39.4	38.0	185	84	39.6	5	741	47	89.0	6.94	-3.0	-6.96	5.62
151											261	20	28.6	1.33			
153	568	992	65.7	118	106	103	542	86	109	7	1831	240	228	9.75	-2.8	-3.97	5.71
156											98.2	15	11.4	0.95			
170 (+190)	30.0	175	12.6	26.6	25.3	24.9	72.4	123	25.6	4	296	16	42.6	2.18	-3.0	-8.84	8.19
180	144	490	30.6	78.2	71.2	69.7	222	108	73.1	6	862	75	138	9.70	-3.0	-4.82	7.19
183	101	136	9.6	22.4	20.8	20.7	82.2	79	21.3	5	234	13	38.0	1.83	-2.6	-7.15	5.29
187	308	419	28.5	66.9	63.2	61.9	252	80	64.0	4	710	72	121	11.1	-2.6	-3.94	5.33
194	8.9	75.9	5.4	31.1	29.3	29.3	30.1	132	29.9	3	127	15	53.5	5.18	-3.1	-4.47	8.81
195	8.06	19.5	1.43	5.46	5.13	5.09	9.67	95	5.23	4	36.8	14.5	14.3	2.17	-2.9	-1.30	6.31
201	109	162	11.4	44.9	42.2	41.9	94.0	81	43.0	4	46.2	4.1	16.8	1.30	4.1	11.46	5.41
206	29.6	47.9	3.5	26.8	24.8	24.8	27.0	83	25.5	5	81.7	13	44.9	4.23	-2.7	-2.84	5.51
209	12.7	14.7	1.1	10.8	10.2	10.3	9.48	78	10.4	3	26.0	5.7	17.2	1.86	-2.5	-1.99	5.17
66	45.2	109	10.8	23.0	23.3	8.3	55.0	90	18.2	47	77.2	40	22.4	0.51	-1.2	-0.37	6.03
95											308	31	33.9	0.51			
														Number by Category			
														Category	z (25%)	z (s)	p (15%)
														≤ 2	3	5	0
														2 to 3	12	3	0
														≥ 3	10	17	26

^aCertified values are in bold ^bSee text for explanation

Certified values are in bold. See text for explanation.

2005 EXERCISE FOR ORGANOCHLORINES IN MARINE MAMMAL TISSUES
 SAMPLES: Homogenate VII AND SRM 1945

Laboratory Number: 18

FATTY ACID ANALYSES			Mass Fraction (%)									
			Homog VII			SRM 1945			Homog VII		SRM 1945	
			Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD	lab mean ng/g wet	lab %RSD
Lauric acid	Dodecanoic acid	C12:0	0.07	0.09	0.09	0.19	0.20	0.19	0.08	8.2	0.19	2.9
Myristic acid	Tetradecanoic acid	C14:0	0.48	0.90	0.78	0.79	0.99	0.83	0.72	30.0	0.87	12.5
Pentadecanoic acid	Pentadecanoic acid	C15:0	0.07	0.08	0.08	0.25	0.26	0.23	0.07	6.6	0.25	5.3
Palmitic acid	Hexadecanoic acid	C16:0	0.65	1.21	1.07	1.09	1.43	1.14	0.98	30.2	1.22	15
Margaric acid	Heptadecanoic acid	C17:0	0.05	0.06	0.06	0.17	0.17	0.15	0.06	6.8	0.16	5.4
Stearic acid	Octadecanoic acid	C18:0	0.58	0.67	0.68	0.83	0.87	0.79	0.65	8.4	0.83	4.9
Arachidic acid	Eicosanoic acid	C20:0	0.08	0.08	0.08	0.08	0.07	0.06	0.08	3.1	0.07	9.6
Palmitoleic acid	(Z)-9-Hexadecanoic acid	C16:1(n-7)	2.82	3.15	3.16	4.95	5.32	4.96	3.04	6.4	5.08	4.1
Vaccenic acid	(Z)-11-Octadecenoic acid	C18:1(n-7)	1.41	1.26	1.25	1.53	1.73	1.50	1.31	6.9	1.59	8.1
Oleic acid	(Z)-9-Octadecanoic acid	C18:1(n-9)	17.48	18.71	18.81	18.06	18.07	17.12	18.3	4.1	17.8	3.1
Elaidic acid	(E)-9-Octadecenoic acid	C18:1(n-9)										
	(Z)-13-eicosenoic acid	C20:1(n-7)										
Gondoic	(Z)-11-eicosenoic acid	C20:1(n-9)	5.49	6.50	6.30	4.18	4.41	4.13	6.09	8.8	4.24	3.5
Gadoleic acid	(Z)-9-Eicosenoic acid	C20:1(n-11)	6.82	5.27	5.65	3.00	3.14	3.02	5.91	13.6	3.05	2.7
Erucic acid	(Z)-13-Docosenoic acid	C22:1(n-9)	0.53	0.82	0.84	0.45	0.56	0.39	0.73	24.1	0.47	17
Cetoleic	(Z)-11-docosenoic acid	C22:1(n-11)	6.01	5.96	5.86	5.23	5.27	4.90	5.94	1.3	5.14	3.9
Nervonic acid	(Z)-15-Tetracosenoic acid	C24:1(n-9)	0.19	0.18	0.20	0.29	0.31	0.29	0.19	4.0	0.29	3.6
Linoleic acid	(Z,Z)-9,12-Octadecadienoic acid	C18:2(n-6)	0.46	0.46	0.49	0.75	0.79	0.73	0.47	3.4	0.75	4.2
a-Linolenic acid	(Z,Z,Z)-9,12,15-Octadecatrienoic acid	C18:3(n-3)	0.43	0.59	0.58	0.34	0.37	0.35	0.54	17.2	0.35	4.9
g-linolenic acid	(Z,Z,Z)-6,9,12-Octadecatetraenoic acid	C18:3(n-6)	0.01	0.01	0.01	0.02	0.02	0.02	0.01	2.8	0.02	4.1
Stearidonic acid	(Z,Z,Z,Z)-6,9,12,15-Octadecatetraenoic acid	C18:4(n-3)	0.08	0.08	0.08	0.20	0.22	0.20	0.08	5.9	0.21	3.5
Homo-gamma-linoleic acid	(Z,Z)-11,14-Eicosadienoic acid	C20:2(n-6)	0.15	0.15	0.15	0.21	0.23	0.22	0.15	1.3	0.22	4.1
Homo-alpha-linolenic acid	(Z,Z,Z)-11,14,17-Eicosatrienoic acid	C20:3(n-3)				0.14	0.15	0.13			0.14	4.8
Arachidonic acid	(Z,Z,Z,Z)-5,8,11,14-Eicosatetraenoic acid	C20:4(n-6)	0.12	0.13	0.14	0.22	0.24	0.23	0.13	4.6	0.23	4.4
EPA	(Z,Z,Z,Z)-5,8,11,14,17-Eicosapentaenoic acid	C20:5(n-3)	0.35	0.39	0.40	1.00	1.20	1.06	0.38	6.9	1.09	9.3
	(Z,Z)-13,16-Docosadienoic acid	C22:2(n-6)	0.03	0.03	0.03	0.03	0.02	0.02	0.03	10.1	0.02	16
DPA	(Z,Z,Z,Z)-7,10,13,16,19-Docosapentaenoic acid	C22:5(n-3)	0.28	0.29	0.31	0.94	1.06	1.01	0.29	3.9	1.00	6.0
DHA	(Z,Z,Z,Z,Z)-4,7,10,13,16,19-Docosahexaenoic Acid	C22:6(n-3)	0.80	0.89	0.88	3.25	3.61	3.16	0.86	5.4	3.34	7.0
Total Lipid			70.3	73.5	83.6	68.1	68.4	69.0	75.8	9.2	68.5	0.7

2005 EXERCISE FOR ORGANOCHLORINES IN MARINE MAMMAL TISSUES
 SAMPLES: Homogenate VII AND SRM 1945

Laboratory Number: 19

FATTY ACID ANALYSES			Mass Fraction (%)											
			Homog VII			SRM 1945			Homog VII		SRM 1945			
			Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean	lab %RSD	lab mean	lab %RSD	ng/g wet	ng/g wet
Lauric acid	Dodecanoic acid	C12:0	0.08	0.08	0.08	0.15	0.15	0.14	0.08	0.00	0.15	3.9		
Myristic acid	Tetradecanoic acid	C14:0	1.53	1.51	1.48	3.20	3.16	3.04	1.51	1.7	3.13	2.7		
Pentadecanoic acid	Pentadecanoic acid	C15:0	0.08	0.07	0.07	0.31	0.31	0.29	0.07	7.9	0.30	3.8		
Palmitic acid	Hexadecanoic acid	C16:0	2.46	2.46	2.41	7.68	7.57	7.27	2.44	1.2	7.51	2.8		
Margaric acid	Heptadecanoic acid	C17:0	0.05	0.04	0.06	0.26	0.21	0.20	0.05	20.0	0.22	14.4		
Stearic acid	Octadecanoic acid	C18:0	0.72	0.72	0.70	1.29	1.26	1.21	0.71	1.6	1.25	3.2		
Arachidic acid	Eicosanoic acid	C20:0	0.15	0.12	0.09	0.11	0.11	0.09	0.12	25.0	0.10	11.2		
Palmitoleic acid	(Z)-9-Hexadecanoic acid	C16:1(n-7)	3.14	3.09	3.03	5.90	5.78	5.56	3.09	1.8	5.75	3.0		
Vaccenic acid	(Z)-11-Octadecenoic acid	C18:1(n-7)	1.30	1.23	1.21	1.83	1.81	1.75	1.25	3.8	1.80	2.3		
Oleic acid	(Z)-9-Octadecanoic acid	C18:1(n-9)	13.60	13.50	13.20	14.20	14.00	13.40	13.4	1.5	13.9	3.0		
Elaidic acid	(E)-9-Octadecenoic acid	C18:1(n-9)	< 0.01	< 0.01	< 0.01	< 0.01	< 0.01	< 0.01						
	(Z)-13-eicosenoic acid	C20:1(n-7)	0.26	0.26	0.27	0.25	0.24	0.23	0.26	2.2	0.24	4.2		
Gondoic	(Z)-11-eicosenoic acid	C20:1(n-9)	7.14	7.14	6.98	4.79	4.71	4.50	7.09	1.3	4.67	3.2		
Gadoleic acid	(Z)-9-Eicosenoic acid	C:20:1(n-11)	5.08	5.08	4.95	3.02	2.96	2.84	5.04	1.5	2.94	3.1		
Erucic acid	(Z)-13-Docosenoic acid	C22:1(n-9)	0.74	0.74	0.72	0.54	0.50	0.50	0.73	1.6	0.51	4.5		
Cetoleic	(Z)-11-docosenoic acid	C22:1(n-11)	4.68	4.70	4.54	4.74	4.63	4.45	4.64	1.9	4.61	3.2		
Nervonic acid	(Z)-15-Tetracosenoic acid	C24:1(n-9)	0.15	0.14	0.15	0.23	0.22	0.21	0.15	3.9	0.22	4.5		
Linoleic acid	(Z,Z)-9,12-Octadecadienoic acid	C18:2(n-6)	0.41	0.41	0.40	0.78	0.76	0.71	0.41	1.4	0.75	4.8		
a-Linolenic acid	(Z,Z,Z)-9,12,15-Octadecatrienoic acid	C18:3(n-3)	0.08	0.09	0.08	0.33	0.33	0.31	0.08	6.9	0.32	3.6		
g-linolenic acid	(Z,Z,Z)-6,9,12-Octadecatetraenoic acid	C18:3(n-6)	0.01	< 0.01	0.01	0.02	0.02	0.02	0.01	0.0	0.02	0.0		
Stearidonic acid	(Z,Z,Z,Z)-6,9,12,15-Octadecatetraenoic acid	C18:4(n-3)	0.15	0.14	0.14	0.24	0.23	0.23	0.14	4.0	0.23	2.5		
Homo-gamma-linoleic acid	(Z,Z)-11,14-Eicosadienoic acid	C20:2(n-6)	0.07	0.06	0.07	0.18	0.17	0.17	0.07	8.7	0.17	3.3		
Homo-alpha-linolenic acid	(Z,Z)-11,14,17-Eicosatrienoic acid	C20:3(n-3)	0.03	0.03	0.03	0.14	0.13	0.13	0.03	0.0	0.13	4.3		
Arachidonic acid	(Z,Z,Z,Z)-5,8,11,14-Eicosatetraenoic acid	C20:4(n-6)	0.11	0.13	0.11	0.23	0.22	0.22	0.12	9.9	0.22	2.6		
EPA	(Z,Z,Z,Z)-5,8,11,14,17-Eicosapentaenoic acid	C20:5(n-3)	0.31	0.32	0.31	1.15	1.12	1.08	0.31	1.8	1.12	3.1		
	(Z,Z)-13,16-Docosadienoic acid	C22:2(n-6)	< 0.01	< 0.01	< 0.01	< 0.01	< 0.01	< 0.01						
DPA	(Z,Z,Z,Z)-7,10,13,16,19-Docosapentaenoic acid	C22:5(n-3)	0.20	0.20	0.20	0.88	0.90	0.85	0.20	0.0	0.88	2.9		
DHA	(Z,Z,Z,Z,Z)-4,7,10,13,16,19-Docosahexaenoic Acid	C22:6(n-3)	0.57	0.57	0.57	3.75	3.71	3.63	0.57	0.0	3.70	1.7		
Total Lipid			81.1	82	78.5	75.9	73.8	66.7	80.5	2.3	72.1	6.7		

2005 EXERCISE FOR ORGANOCHLORINES IN MARINE MAMMAL TISSUES
 SAMPLES: Homogenate VII AND SRM 1945

Laboratory Number: 20

FATTY ACID ANALYSES			Mass Fraction (%)									
			Homog VII			SRM 1945			Homog VII		SRM 1945	
			Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean	lab %RSD	lab mean	lab %RSD
Lauric acid	Dodecanoic acid	C12:0	0.06	0.08	0.07	0.14	0.12	0.12	0.07	14.0	0.13	8.4
Myristic acid	Tetradecanoic acid	C14:0	1.19	1.33	1.41	2.73	2.81	2.60	1.31	8.6	2.71	3.8
Pentadecanoic acid	Pentadecanoic acid	C15:0	0.05	0.05	0.06	0.24	0.22	0.22	0.05	4.7	0.23	4.8
Palmitic acid	Hexadecanoic acid	C16:0	1.78	2.04	2.19	5.86	6.17	5.86	2.00	10.2	5.96	3.0
Margaric acid	Heptadecanoic acid	C17:0	0.04	0.03	0.04	0.16	0.18	0.15	0.04	12.6	0.16	6.6
Stearic acid	Octadecanoic acid	C18:0	0.48	0.63	0.71	1.09	1.18	1.06	0.61	19.3	1.11	5.4
Arachidic acid	Eicosanoic acid	C20:0	0.05	0.05	0.04	0.09	0.06	0.07	0.05	12.4	0.07	22.0
Palmitoleic acid	(Z)-9-Hexadecanoic acid	C16:1(n-7)	2.34	2.72	2.96	4.60	4.42	4.48	2.67	11.5	4.50	2.0
Vaccenic acid	(Z)-11-Octadecenoic acid	C18:1(n-7)	0.99	1.19	1.32	1.62	1.60	1.61	1.17	14.0	1.61	0.5
Oleic acid	(Z)-9-Octadecenoic acid	C18:1(n-9)	8.00	10.46	11.68	10.86	11.94	10.03	10.0	18.6	10.9	8.8
Elaidic acid	(E)-9-Octadecenoic acid	C18:1(n-9)										
	(Z)-13-eicosenoic acid	C20:1(n-7)	0.25	0.29	0.37	0.13	0.24	0.16	0.30	20.3	0.18	31.6
Gondoic	(Z)-11-eicosenoic acid	C20:1(n-9)	4.62	5.70	6.00	3.44	3.71	3.47	5.44	13.3	3.54	4.2
Gadoleic acid	(Z)-9-Eicosenoic acid	C20:1(n-11)	3.32	4.51	4.88	2.32	2.89	2.23	4.24	19.2	2.48	14.4
Erucic acid	(Z)-13-Docosenoic acid	C22:1(n-9)	0.42	0.59	0.69	0.41	0.46	0.46	0.57	24.2	0.44	6.1
Cetoleic	(Z)-11-docosenoic acid	C22:1(n-11)	3.06	3.48	4.01	3.41	3.71	2.85	3.52	13.5	3.32	13.0
Nervonic acid	(Z)-15-Tetracosenoic acid	C24:1(n-9)	0.08	0.07	0.08	0.14	0.14	0.10	0.08	9.7	0.13	19.2
Linoleic acid	(Z,Z)-9,12-Octadecadienoic acid	C18:2(n-6)	0.03	0.04	0.03	0.13	0.09	0.11	0.03	17.1	0.11	20.6
a-Linolenic acid	(Z,Z,Z)-9,12,15-Octadecatrienoic acid	C18:3(n-3)										
g-linolenic acid	(Z,Z,Z)-6,9,12-Octadecatetraenoic acid	C18:3(n-6)										
Stearidonic acid	(Z,Z,Z,Z)-6,9,12,15-Octadecatetraenoic acid	C18:4(n-3)										
Homo-gamma-linoleic acid	(Z,Z)-11,14-Eicosadienoic acid	C20:2(n-6)										
Homo-alpha-linolenic acid	(Z,Z,Z)-11,14,17-Eicosatrienoic acid	C20:3(n-3)										
Arachidonic acid	(Z,Z,Z,Z)-5,8,11,14-Eicosatetraenoic acid	C20:4(n-6)	0.04	0.04	0.04	0.08	0.08	0.07	0.04	5.9	0.08	10.5
EPA	(Z,Z,Z,Z)-5,8,11,14,17-Eicosapentaenoic acid	C20:5(n-3)	0.11	0.14	0.15	0.58	0.55	0.49	0.13	17.0	0.54	9.0
	(Z,Z)-13,16-Docosadienoic acid	C22:2(n-6)										
DPA	(Z,Z,Z,Z)-7,10,13,16,19-Docosapentaenoic acid	C22:5(n-3)	0.08	0.09	0.09	0.58	0.47	0.39	0.09	6.0	0.48	20.7
DHA	(Z,Z,Z,Z,Z)-4,7,10,13,16,19-Docosahexaenoic Acid	C22:6(n-3)	0.10	0.13	0.12	0.94	0.95	0.76	0.12	13.4	0.88	12.1
Total Lipid			65.3	72.2	79.7	70.3	69.3	68.6	72.4	9.9	69.4	1.2

2005 EXERCISE FOR ORGANOCHLORINES IN MARINE MAMMAL TISSUES
 SAMPLES: Homogenate VII AND SRM 1945

Laboratory Number: 21

FATTY ACID ANALYSES			Mass Fraction (%)							
			Homog VII			SRM 1945			Homog VII	
			Sample 1	Sample 2	Sample 3	Sample 1	Sample 2	Sample 3	lab mean ng/g wet	lab %RSD
Lauric acid	Dodecanoic acid	C12:0	0.09	0.09	0.09	0.19			0.09	0.7
Myristic acid	Tetradecanoic acid	C14:0	1.72	1.76	1.73	3.63			1.74	1.2
Pentadecanoic acid	Pentadecanoic acid	C15:0	0.08	0.09	0.08	0.36			0.08	1.6
Palmitic acid	Hexadecanoic acid	C16:0	2.64	2.73	2.68	7.41			2.68	1.7
Margaric acid	Heptadecanoic acid	C17:0	0.07	0.07	0.07	0.25			0.07	2.7
Stearic acid	Octadecanoic acid	C18:0	0.89	0.90	0.88	1.43			0.89	1.5
Arachidic acid	Eicosanoic acid	C20:0	0.16	0.17	0.16	0.14			0.17	1.4
Palmitoleic acid	(Z)-9-Hexadecanoic acid	C16:1(n-7)	3.54	3.56	3.64	6.46			3.58	1.5
Vaccenic acid	(Z)-11-Octadecenoic acid	C18:1(n-7)	1.49	1.50	1.47	2.00			1.49	1.0
Oleic acid	(Z)-9-Octadecanoic acid	C18:1(n-9)	15.20	15.20	15.10	15.20			15.2	0.4
Elaidic acid	(E)-9-Octadecenoic acid	C18:1(n-9)								
	(Z)-13-eicosenoic acid	C20:1(n-7)	0.35	0.36	0.34	0.27			0.35	2.2
Gondoic	(Z)-11-eicosenoic acid	C20:1(n-9)	8.17	8.30	8.07	5.27			8.18	1.4
Gadoleic acid	(Z)-9-Eicosenoic acid	C20:1(n-11)	5.69	5.76	5.60	3.25			5.68	1.4
Erucic acid	(Z)-13-Docosenoic acid	C22:1(n-9)	1.11	1.12	1.07	0.80			1.10	2.4
Cetoleic	(Z)-11-docosenoic acid	C22:1(n-11)	5.41	5.51	5.37	5.17			5.43	1.3
Nervonic acid	(Z)-15-Tetracosenoic acid	C24:1(n-9)	0.20	0.20	0.20	0.30			0.20	1.5
Linoleic acid	(Z,Z)-9,12-Octadecadienoic acid	C18:2(n-6)	0.54	0.54	0.53	0.91			0.54	1.1
a-Linolenic acid	(Z,Z,Z)-9,12,15-Octadecatrienoic acid	C18:3(n-3)	0.17	0.17	0.17	0.40			0.17	2.1
g-linolenic acid	(Z,Z,Z)-6,9,12-Octadecatetraenoic acid	C18:3(n-6)	0.02	0.02	0.02	0.03			0.02	4.3
Stearidonic acid	(Z,Z,Z,Z)-6,9,12,15-Octadecatetraenoic acid	C18:4(n-3)	0.09	0.10	0.10	0.20			0.10	6.3
Homo-gamma-linoleic acid	(Z,Z)-11,14-Eicosadienoic acid	C20:2(n-6)	0.17	0.18	0.17	0.03			0.17	2.3
Homo-alpha-linolenic acid	(Z,Z,Z)-11,14,17-Eicosatrienoic acid	C20:3(n-3)	0.07	0.07	0.06	0.19			0.07	3.7
Arachidonic acid	(Z,Z,Z,Z)-5,8,11,14-Eicosatetraenoic acid	C20:4(n-6)	0.18	0.21	0.18	0.31			0.19	8.0
EPA	(Z,Z,Z,Z)-5,8,11,14,17-Eicosapentaenoic acid	C20:5(n-3)	0.51	0.51	0.49	1.27			0.50	1.8
DPA	(Z,Z)-13,16-Docosadienoic acid	C22:2(n-6)	0.03	0.04	0.03	0.04			0.04	18.5
DHA	(Z,Z,Z,Z)-7,10,13,16,19-Docosapentaenoic acid	C22:5(n-3)	0.47	0.29	0.39	0.94			0.38	24.4
Total Lipid	(Z,Z,Z,Z)-4,7,10,13,16,19-Docosahexaenoic Acid	C22:6(n-3)	0.85	0.83	0.83	4.33			0.84	1.5
			71.6	69.3	70.6	61.9			70.5	1.6
										61.9

Appendix B

Graphical results of PCB congener and lipid data reported by all laboratories. The Z-scores for Homogenate VII represent 25 % of the assigned value so that z = +1 is the assigned value plus 25 %, z = -1 is the assigned value minus 25 % and so forth. Error bars are \pm 1 standard deviation.


PCB 18

Assigned value = 6.57 ng/g SD = 13 ng/g 95% CI = \pm 13 ng/g (wet basis)

Reported Results: 8 Quantitative Results: 4

Homogenate VII (Blainville's Beaked Whale)

— Assigned Value
- - - \pm 1 Z
- - - - \pm 2 Z
- - - - - \pm 3 Z

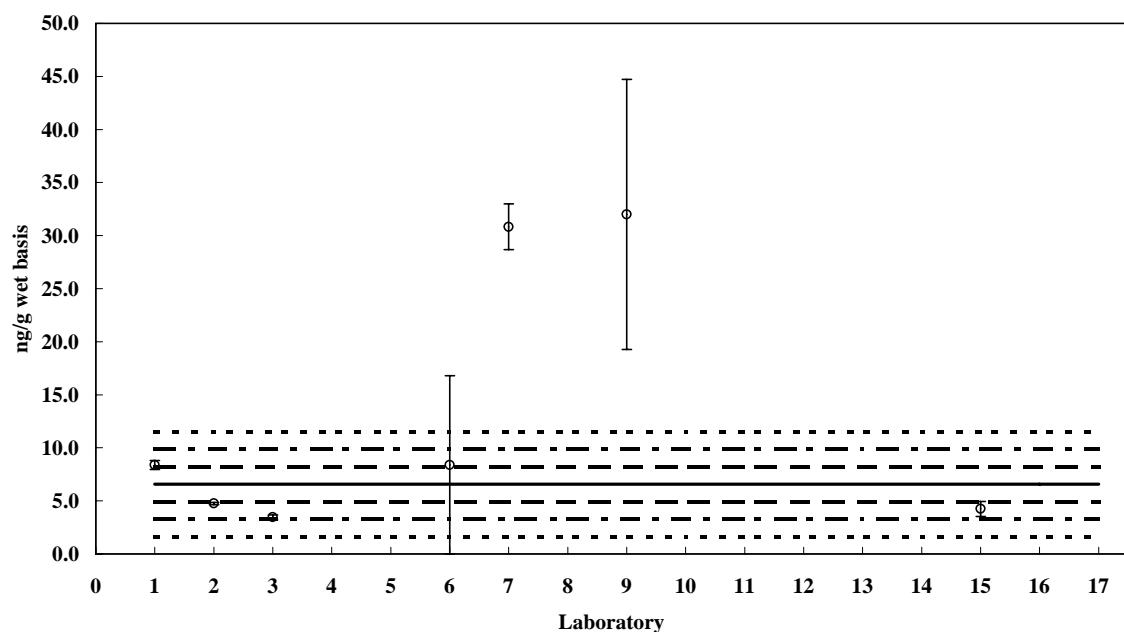

PCB 18

Value = 4.4 ± 0.56 ng/g (wet basis)


Reported Results: 8

SRM 1945

— Certified or Reference Value

- - - \pm Uncertainty

..... \pm 30 % of Certified or Reference Value

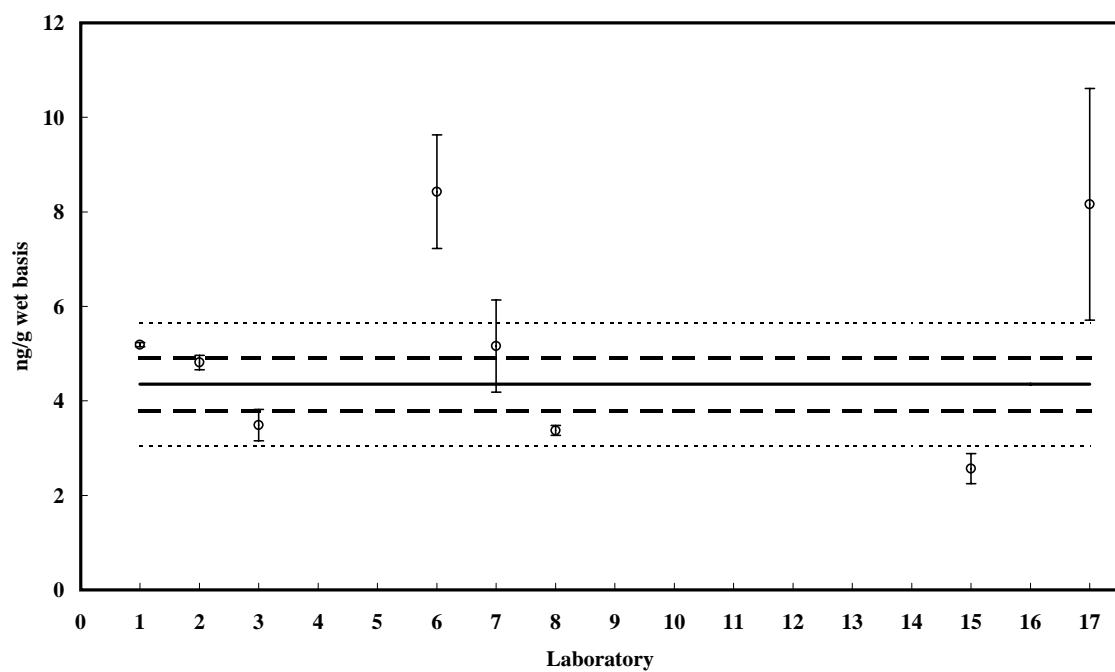


PCB 28Assigned value = 18.6 ng/g SD = 3.6 ng/g 95% CI = \pm 2.4 ng/g (wet basis)

Reported Results: 11 Quantitative Results: 9

Homogenate VII (Blainville's Beaked Whale)


Assigned Value
 \pm 1 Z
 \pm 2 Z
 \pm 3 Z

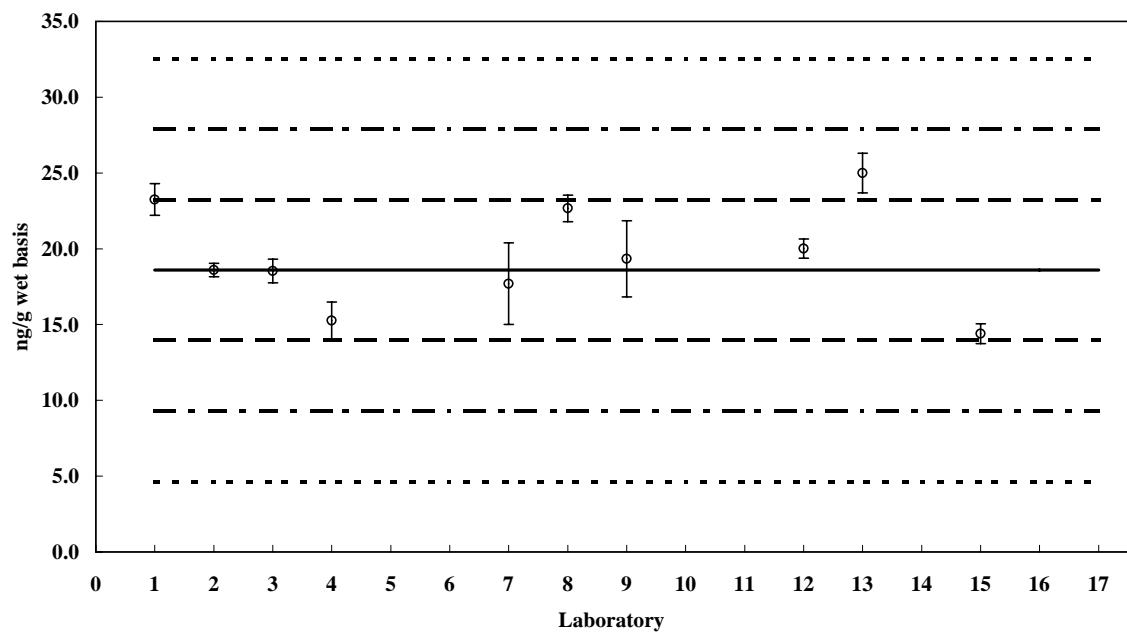**PCB 28**Value = 13 \pm 1 ng/g (wet basis)

Reported Results: 10

SRM 1945

Certified or Reference Value
 \pm Uncertainty
 \pm 30 % of Certified or Reference Value

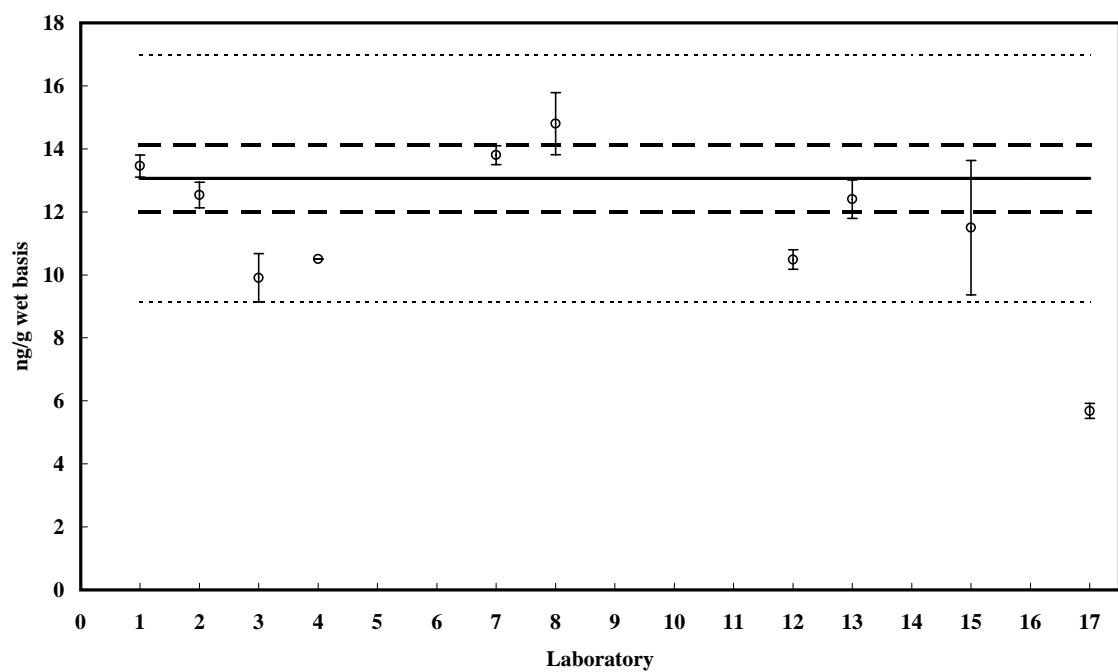


PCB 31Assigned value = 1.76 ng/g SD = 0.66 ng/g 95% CI = \pm 0.74 ng/g (wet basis)

Reported Results: 5 Quantitative Results: 3

Homogenate VII (Blainville's Beaked Whale)


Assigned Value
 \pm 1 Z
 \pm 2 Z
 \pm 3 Z

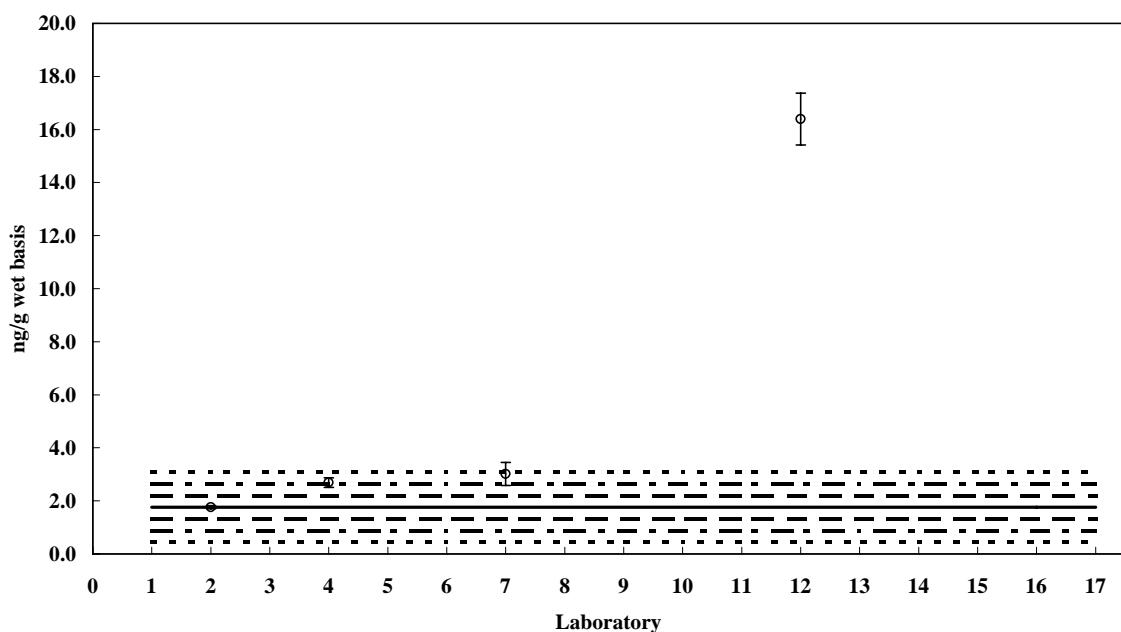**PCB 31**Value = 3.6 \pm 0.4 ng/g (wet basis)

Reported Results: 9

SRM 1945

Certified or Reference Value

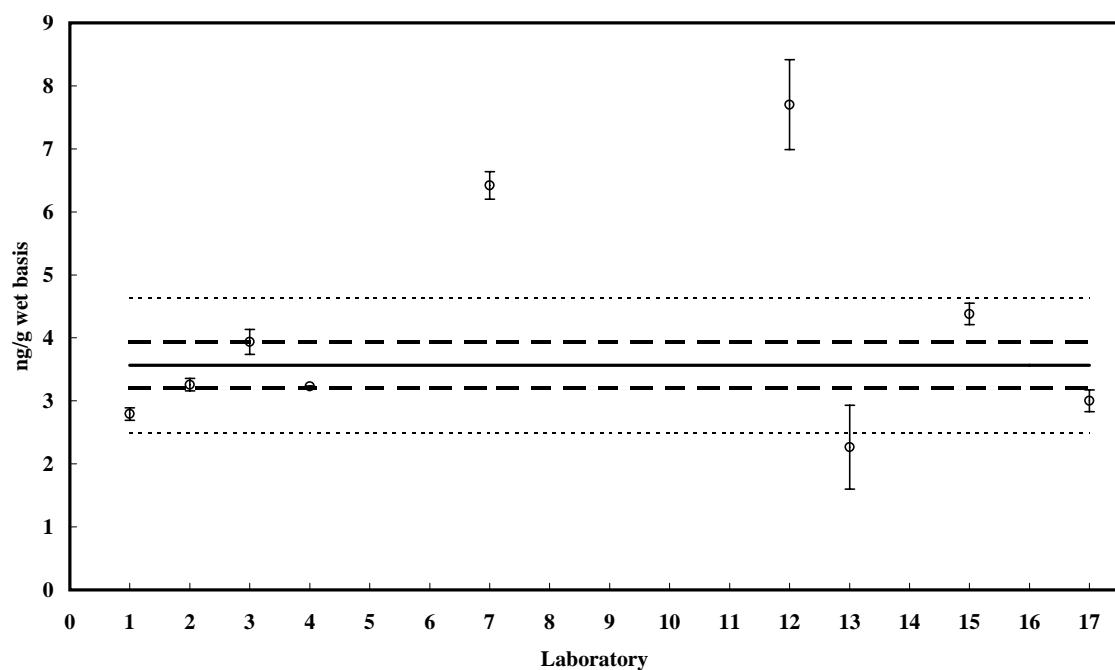 \pm Uncertainty \pm 30 % of Certified or Reference Value


PCB 44

Assigned value = 46.2 ng/g SD = 4.2 ng/g 95% CI = \pm 3.1 ng/g (wet basis)

Reported Results: 10 Quantitative Results: 7

Homogenate VII (Blainville's Beaked Whale)

Assigned Value
 \pm 1 Z
 \pm 2 Z
 \dots \pm 3 Z

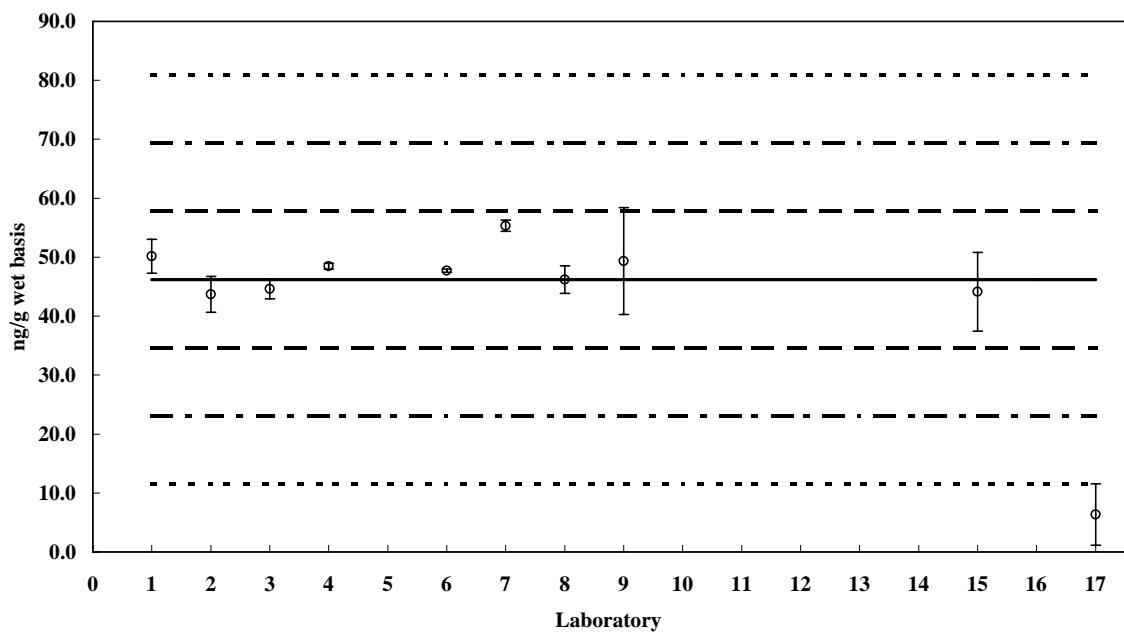

PCB 44

Value = 12.1 \pm 0.51 ng/g (wet basis)


Reported Results: 9

SRM 1945

Certified or Reference Value

\pm Uncertainty

\dots \pm 30 % of Certified or Reference Value

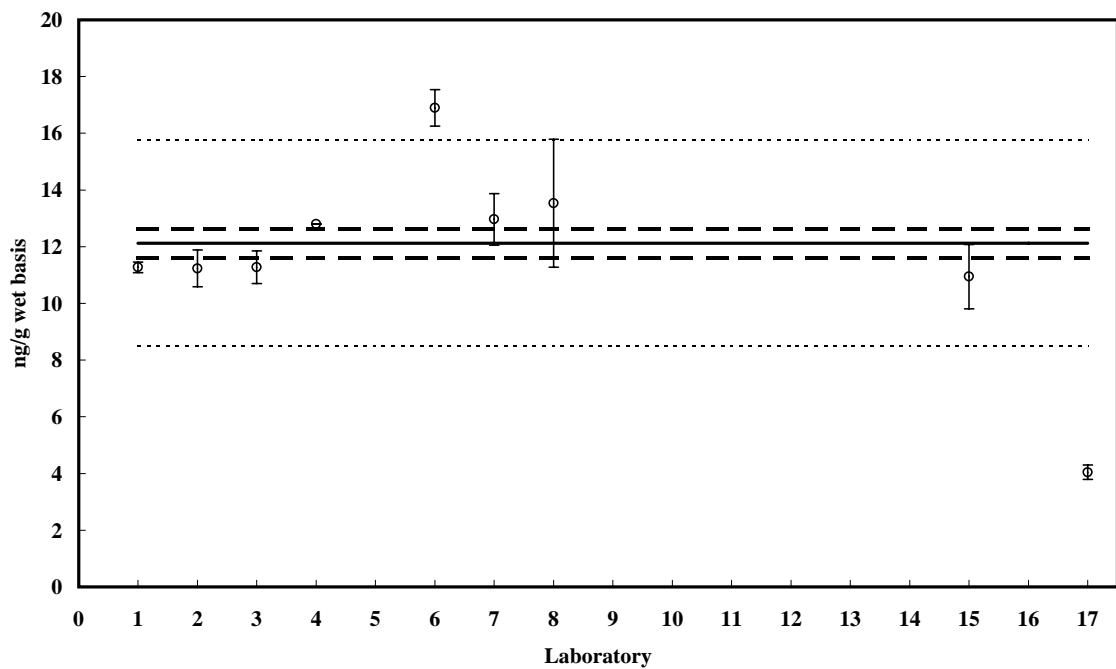


PCB 49

Assigned value = 88.7 ng/g SD = 9.5 ng/g 95% CI = \pm 7.0 ng/g (wet basis)

Reported Results: 10 Quantitative Results: 7

Homogenate VII (Blainville's Beaked Whale)

____ Assigned Value
- - - \pm 1 Z
- - - \pm 2 Z
- - - - \pm 3 Z

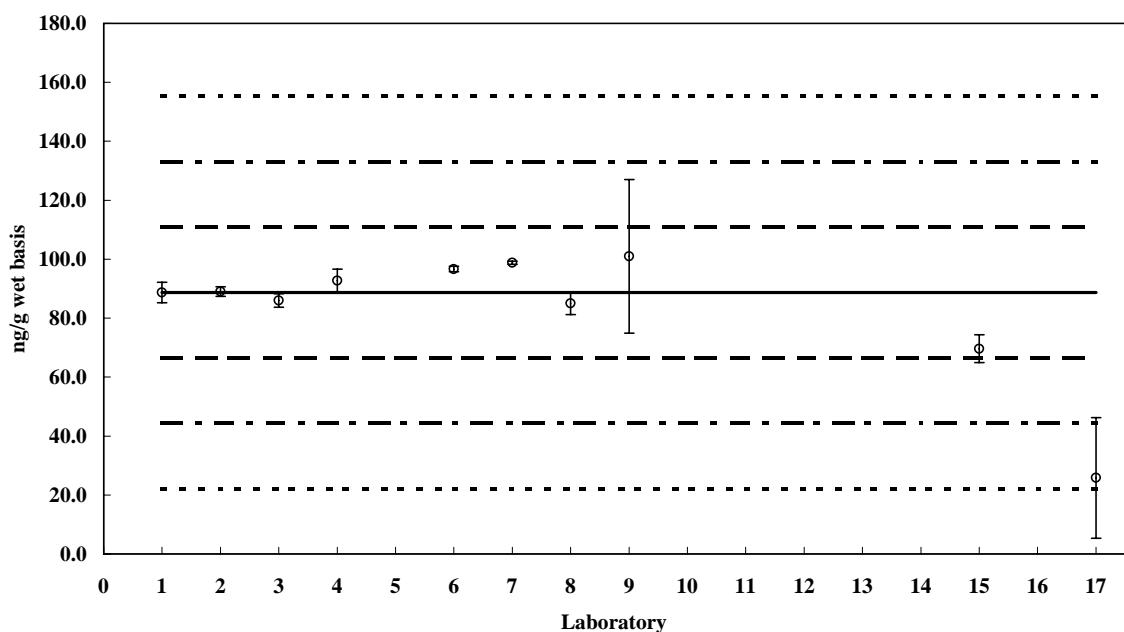

PCB 49

Value = 18.3 \pm 0.1 ng/g (wet basis)


Reported Results: 10

SRM 1945

— Certified or Reference Value

- - - \pm Uncertainty

- - - - \pm 30 % of Certified or Reference Value

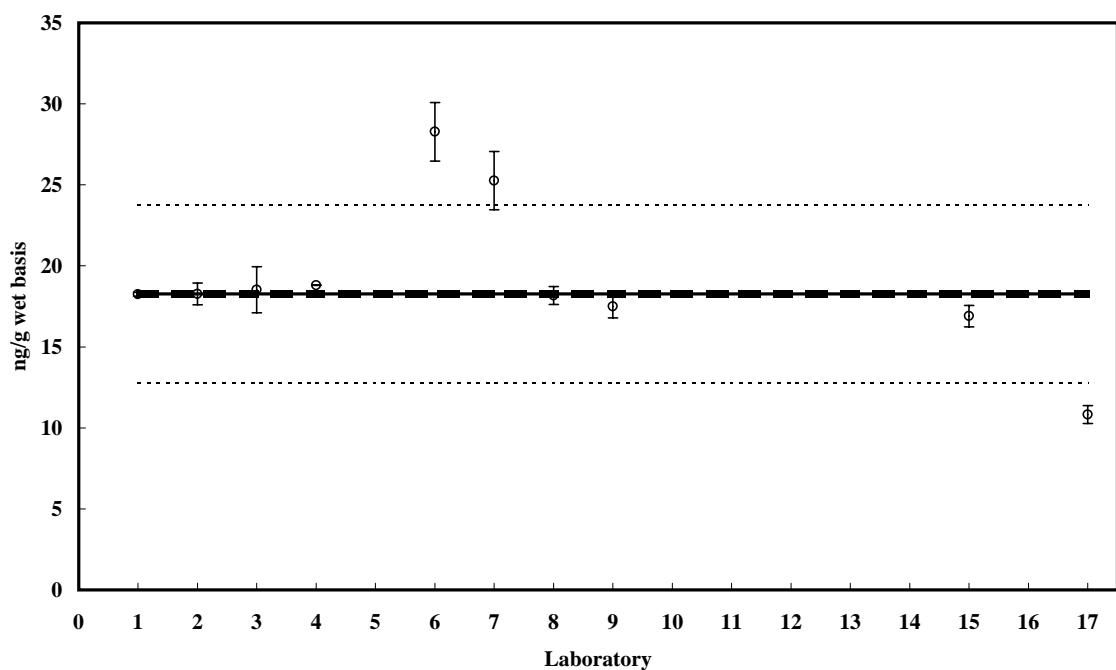


PCB 52Assigned value = 271 ng/g SD = 34 ng/g 95% CI = \pm 20 ng/g (wet basis)

Reported Results: 12 Quantitative Results: 11

Homogenate VII (Blainville's Beaked Whale)


____ Assigned Value
 - - - \pm 1 Z
 - - - \pm 2 Z
 - - - - \pm 3 Z

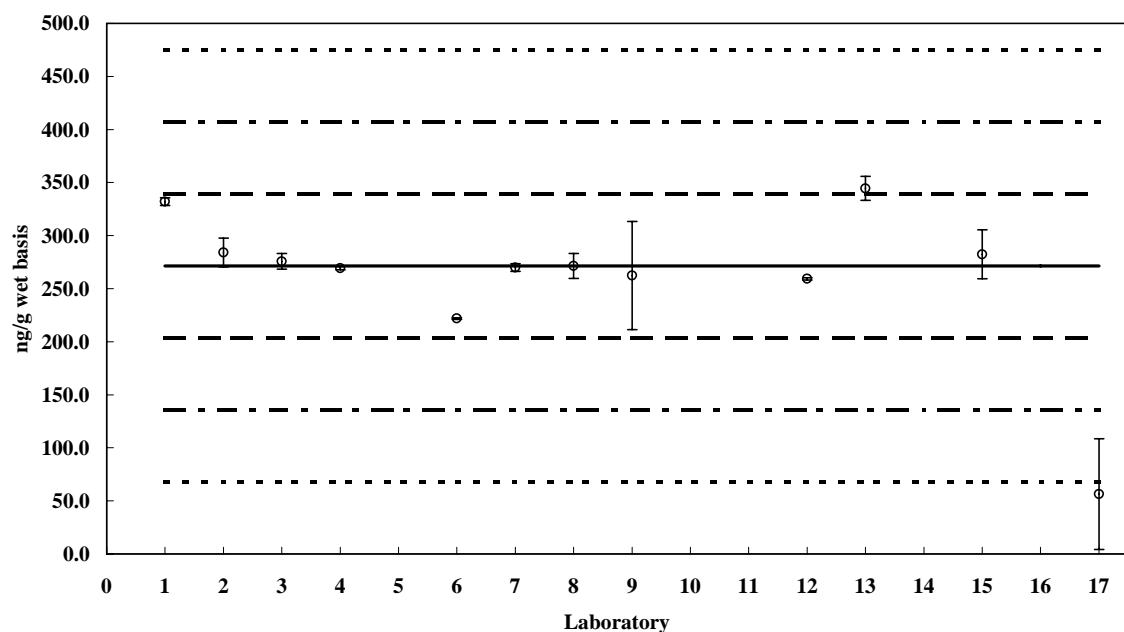**PCB 52**Value = 40.7 \pm 1.3 ng/g (wet basis)

Reported Results: 12

SRM 1945

____ Certified or Reference Value

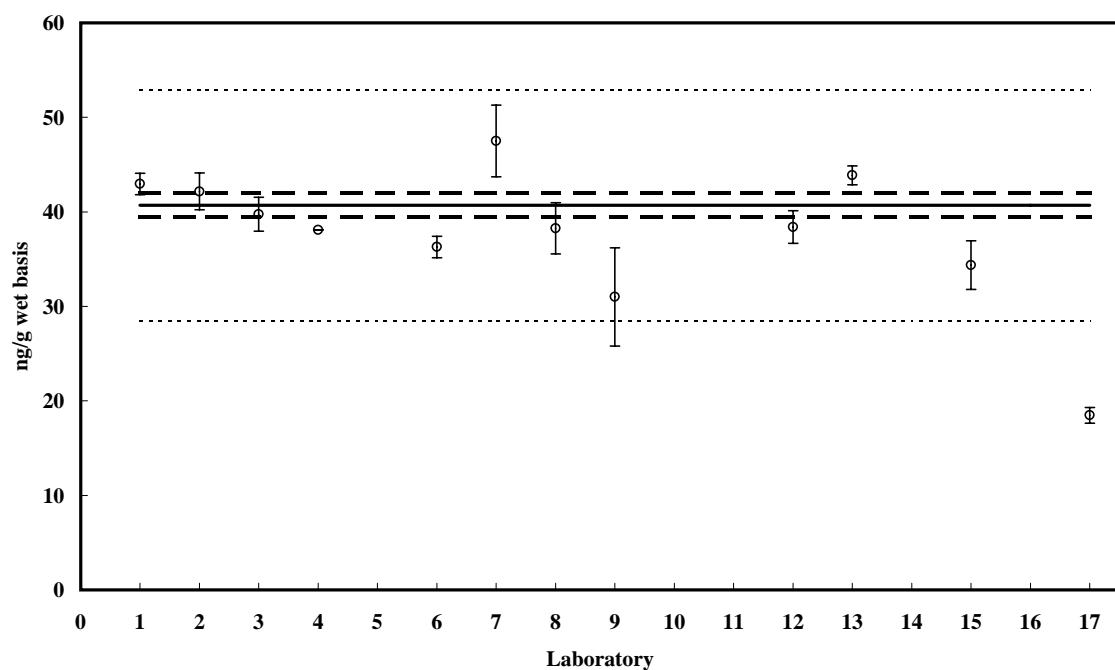- - - \pm Uncertainty- - - - \pm 30 % of Certified or Reference Value


PCB 87

Assigned value = 201 ng/g SD = 16 ng/g 95% CI = \pm 18 ng/g (wet basis)

Reported Results: 5 Quantitative Results: 3

Homogenate VII (Blainville's Beaked Whale)

____ Assigned Value
- - - \pm 1 Z
- - - \pm 2 Z
- - - - \pm 3 Z

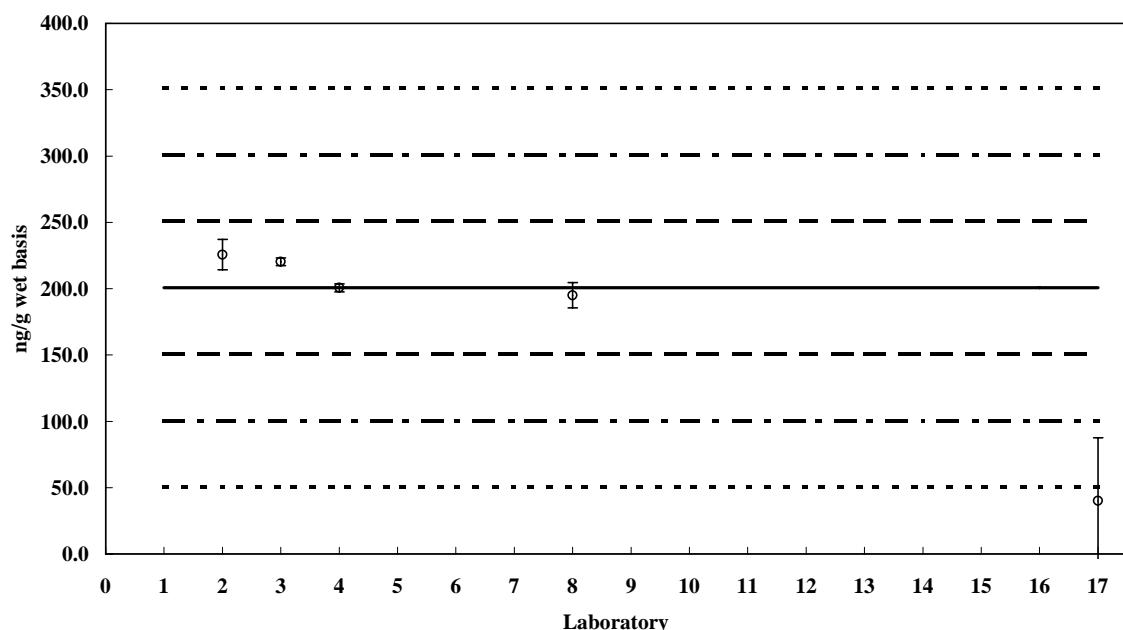

PCB 87

Value = 20.6 \pm 2.6 ng/g (wet basis)


Reported Results: 5



SRM 1945



____ Certified or Reference Value

- - - \pm Uncertainty

..... \pm 30 % of Ceritifed or Reference Value

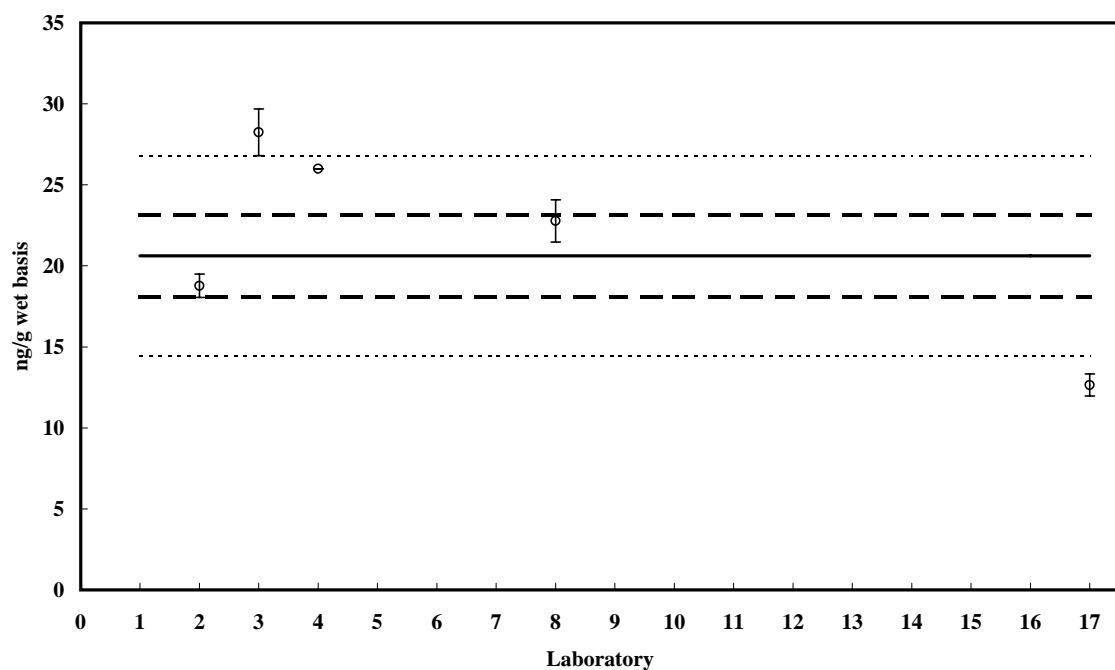

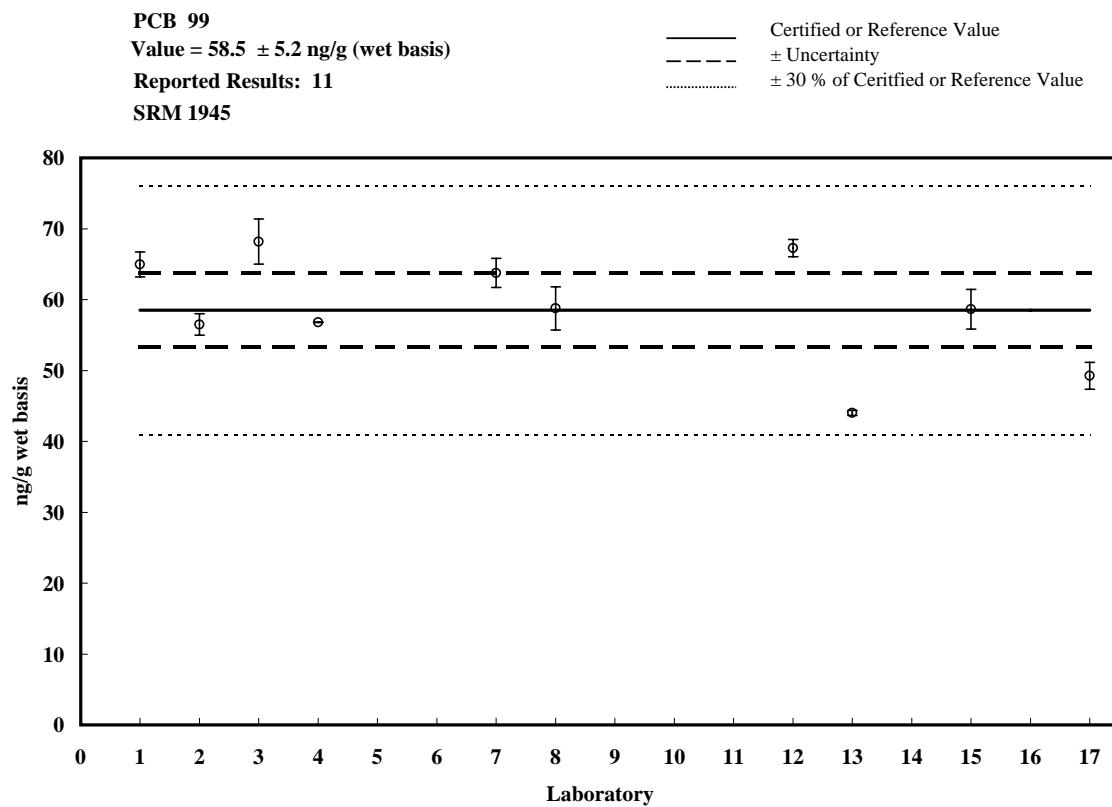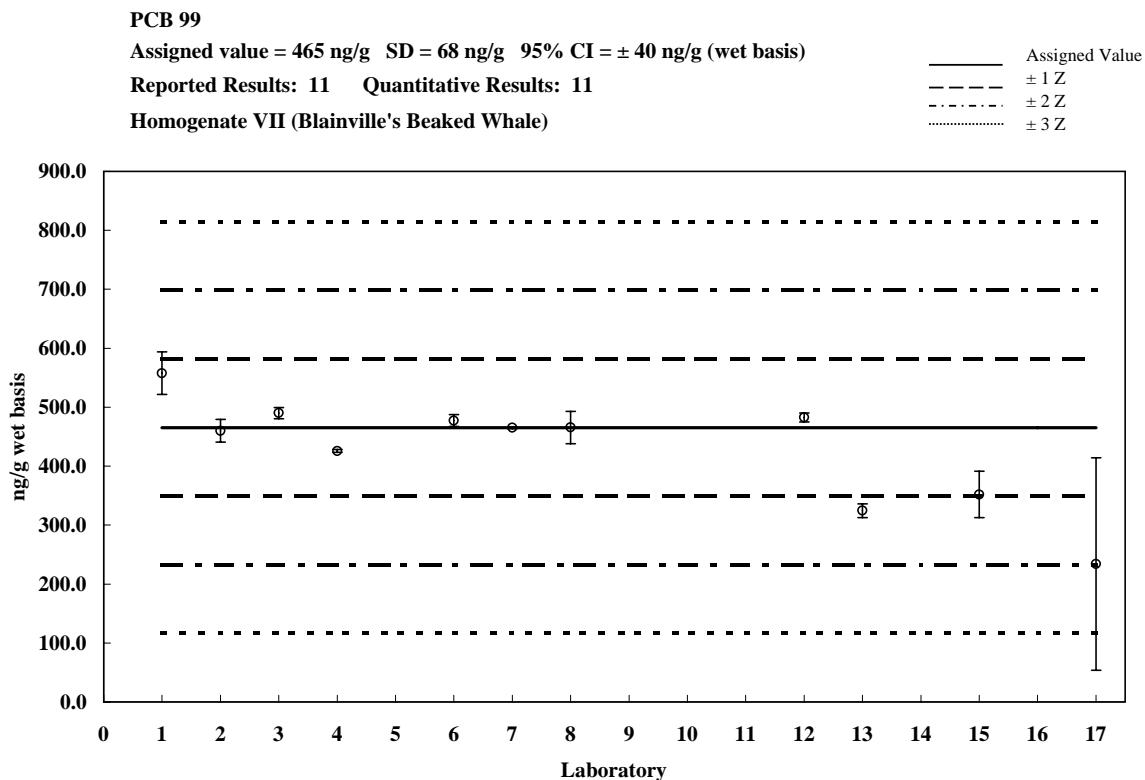

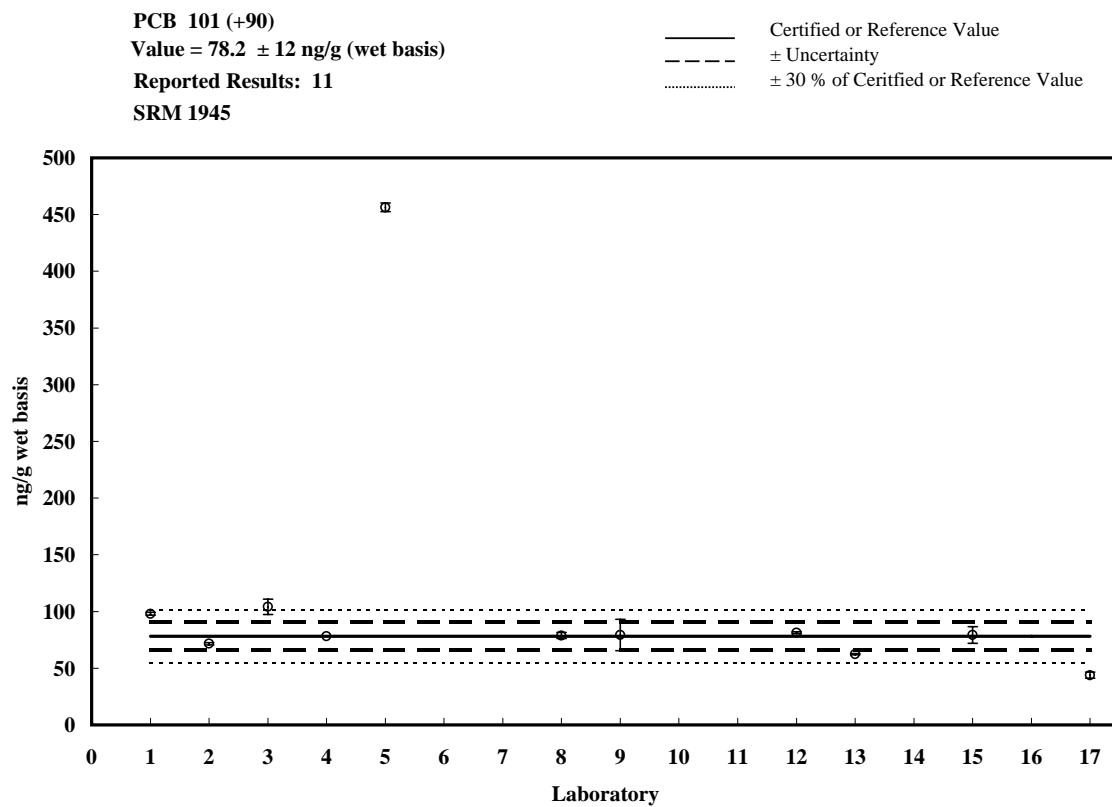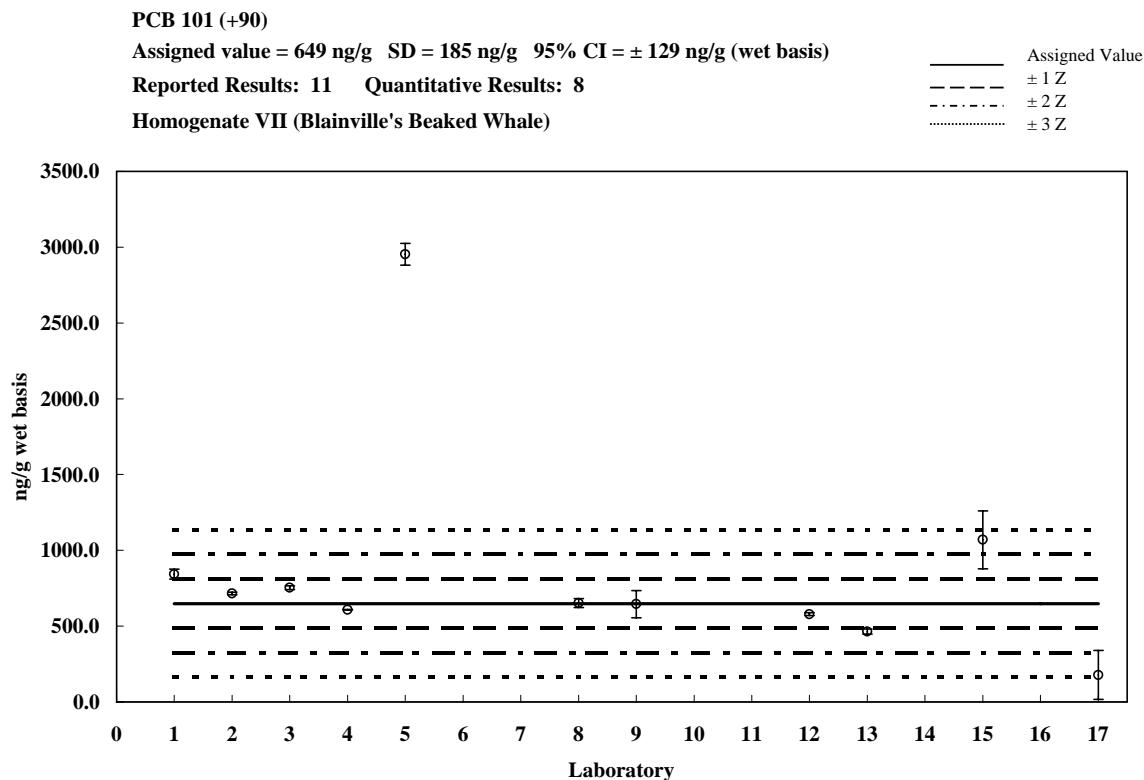


PCB 105

Assigned value = 90.3 ng/g SD = 27 ng/g 95% CI = \pm 16 ng/g (wet basis)

Reported Results: 13 Quantitative Results: 11

Homogenate VII (Blainville's Beaked Whale)

— Assigned Value
- - - \pm 1 Z
- - - \pm 2 Z
- - - - \pm 3 Z

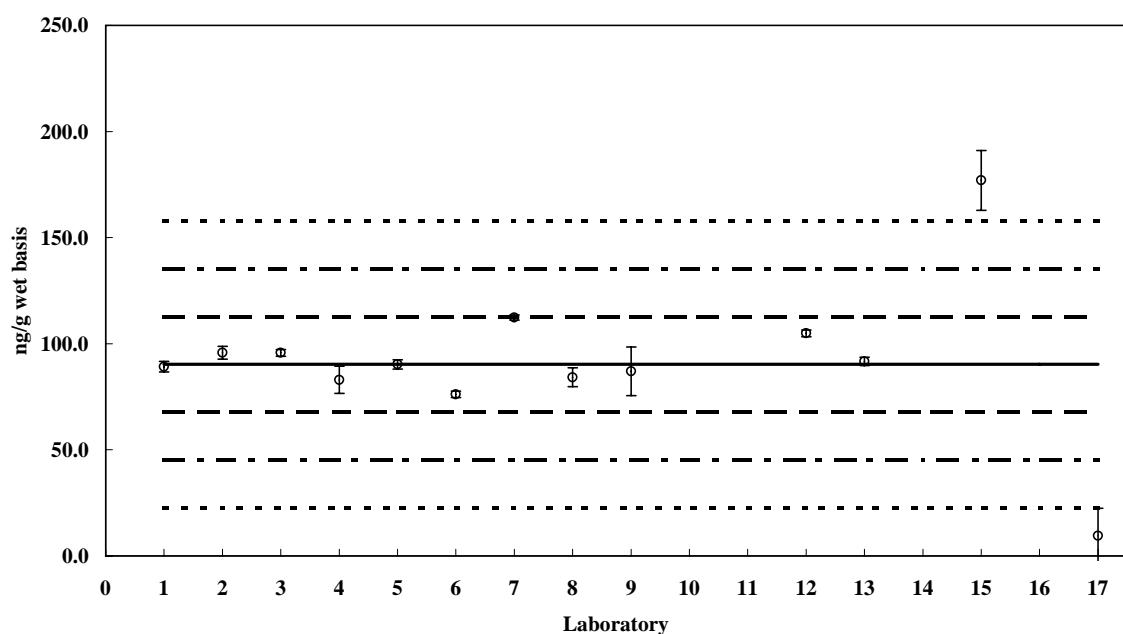

PCB 105

Value = 28.6 \pm 1.2 ng/g (wet basis)


Reported Results: 13

SRM 1945

— Certified or Reference Value

- - - \pm Uncertainty

- - - - \pm 30 % of Certified or Reference Value

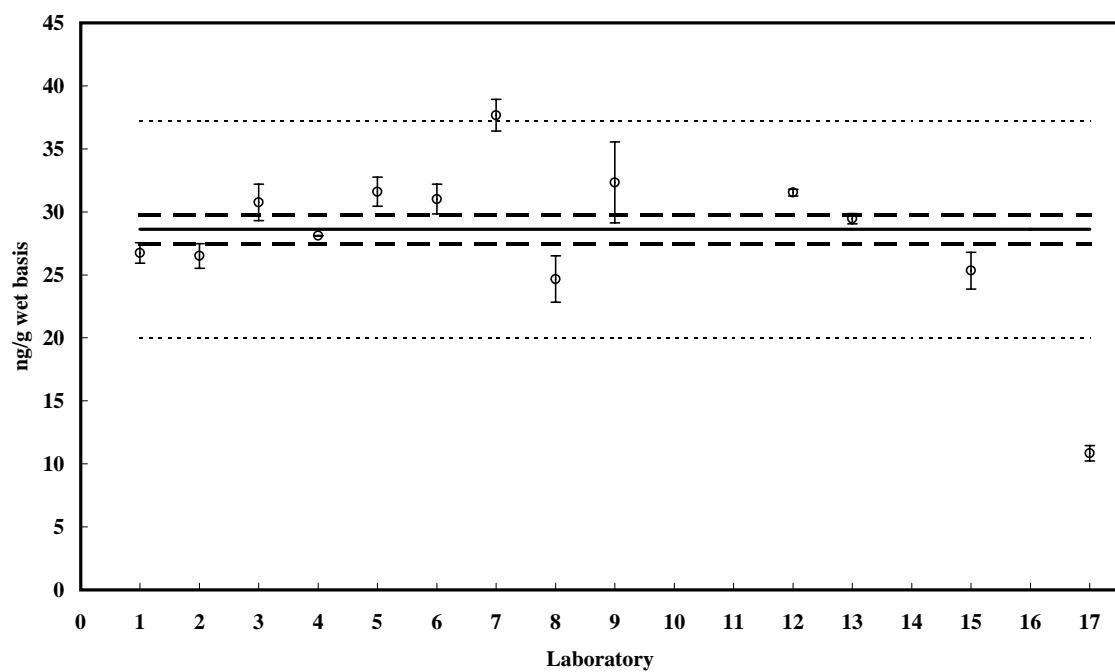


PCB 118Assigned value = 640 ng/g SD = 82 ng/g 95% CI = \pm 51 ng/g (wet basis)

Reported Results: 12 Quantitative Results: 10

Homogenate VII (Blainville's Beaked Whale)


____ Assigned Value
 - - - \pm 1 Z
 - - - \pm 2 Z
 - - - \pm 3 Z


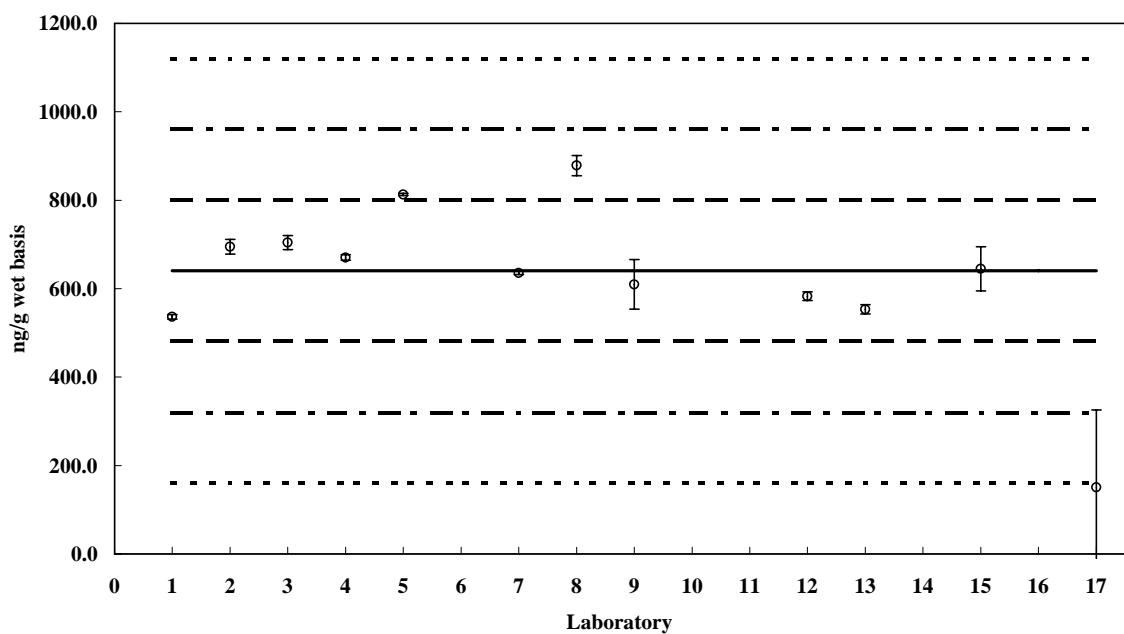
**PCB 118**Value = 76.5 \pm 2.9 ng/g (wet basis)



Reported Results: 12

SRM 1945

____ Certified or Reference Value
 - - - \pm Uncertainty
 - - - \pm 30 % of Certified or Reference Value

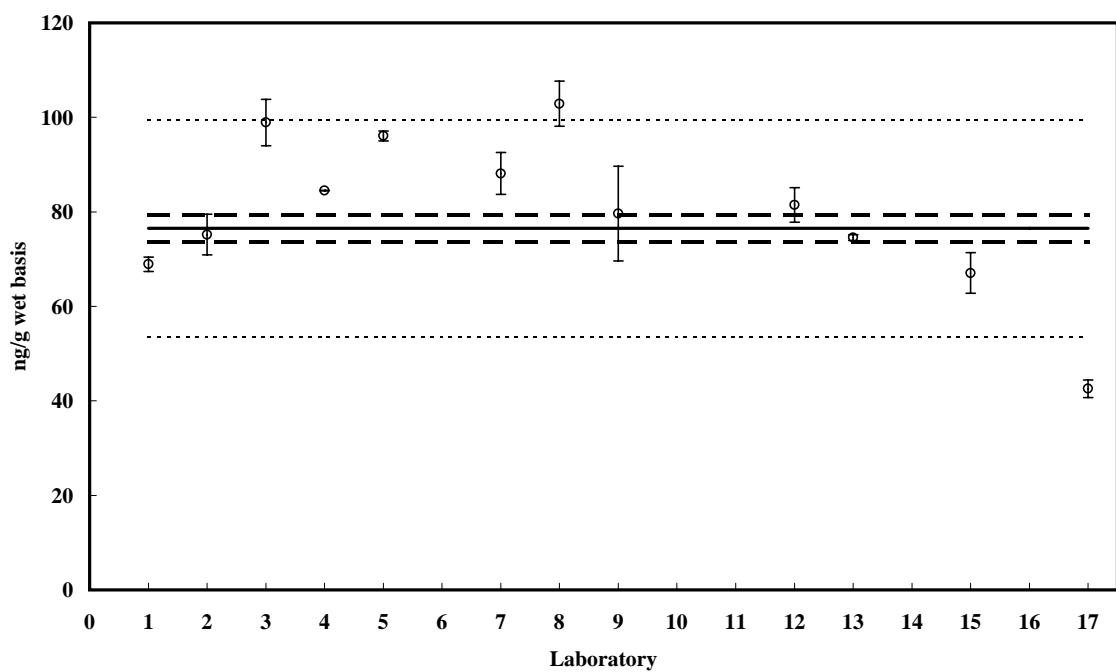

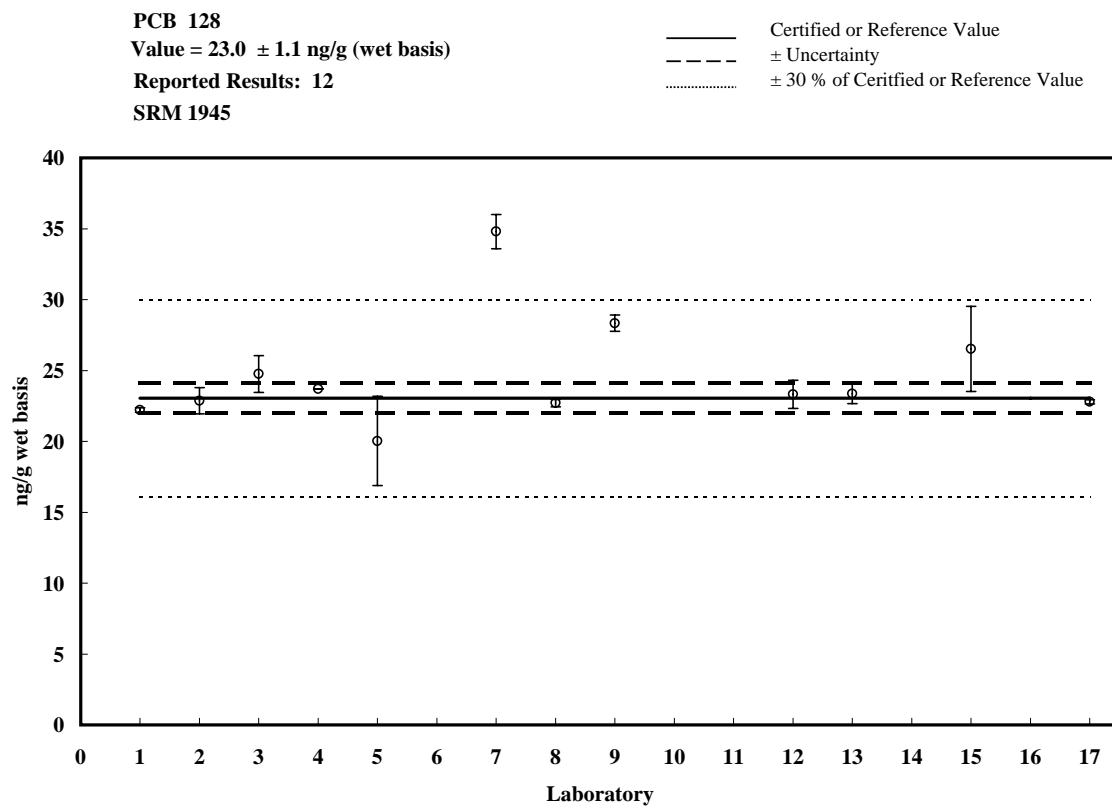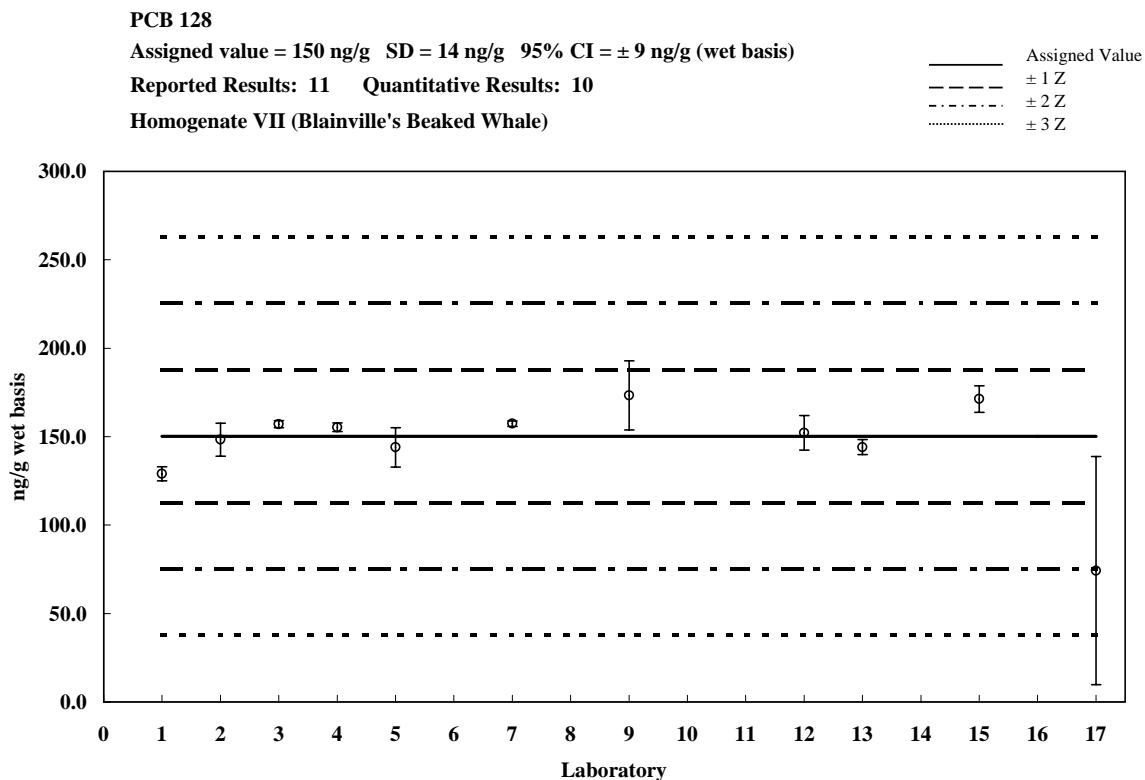

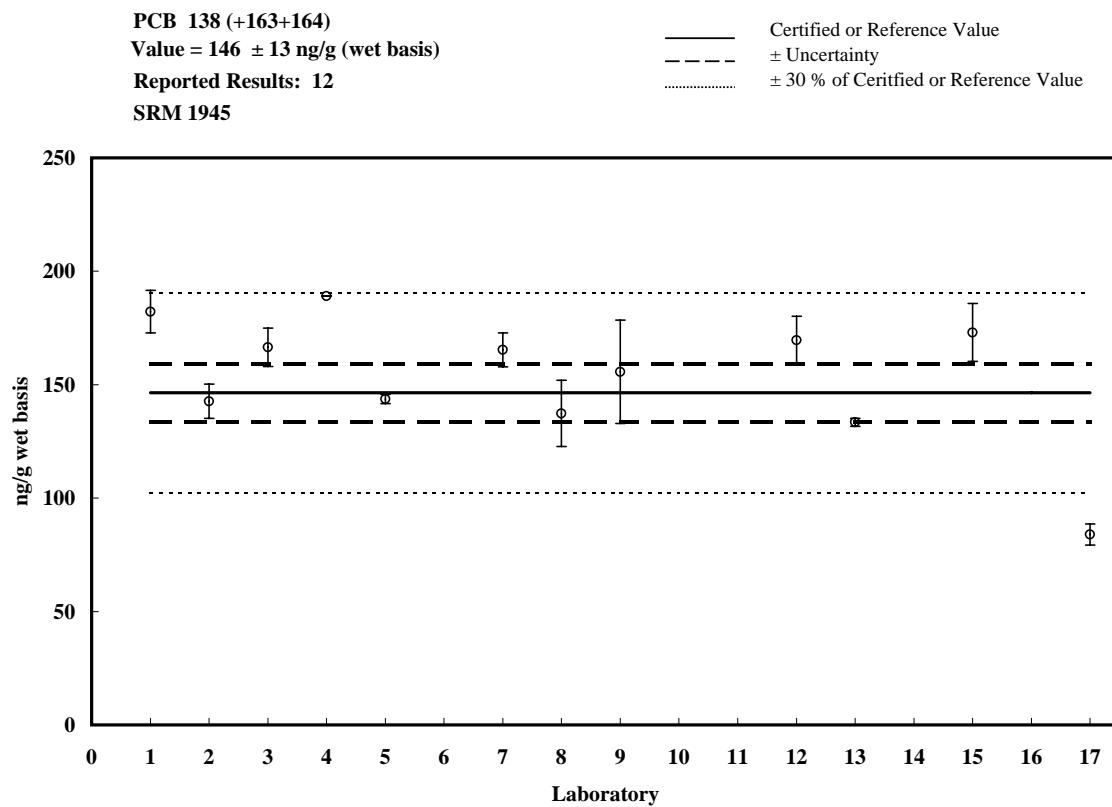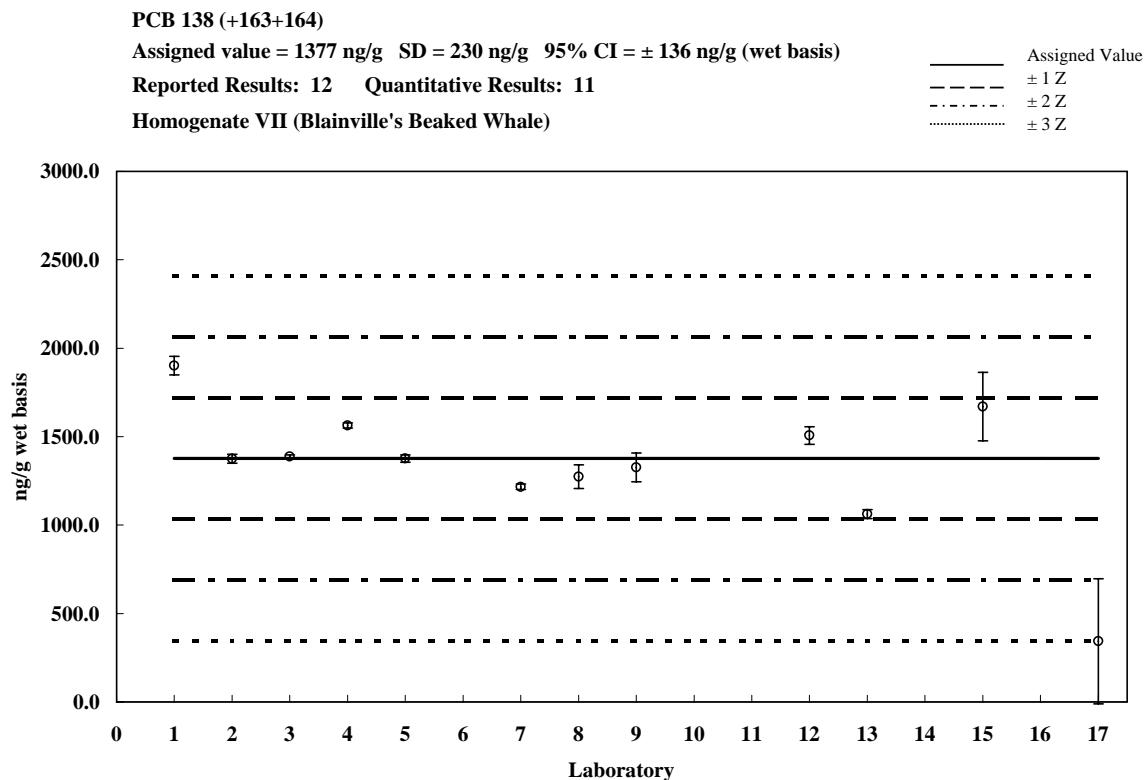


PCB 149Assigned value = 741 ng/g SD = 80 ng/g 95% CI = \pm 47 ng/g (wet basis)

Reported Results: 12 Quantitative Results: 11

Homogenate VII (Blainville's Beaked Whale)


Assigned Value
 \pm 1 Z
 \pm 2 Z
 \pm 3 Z

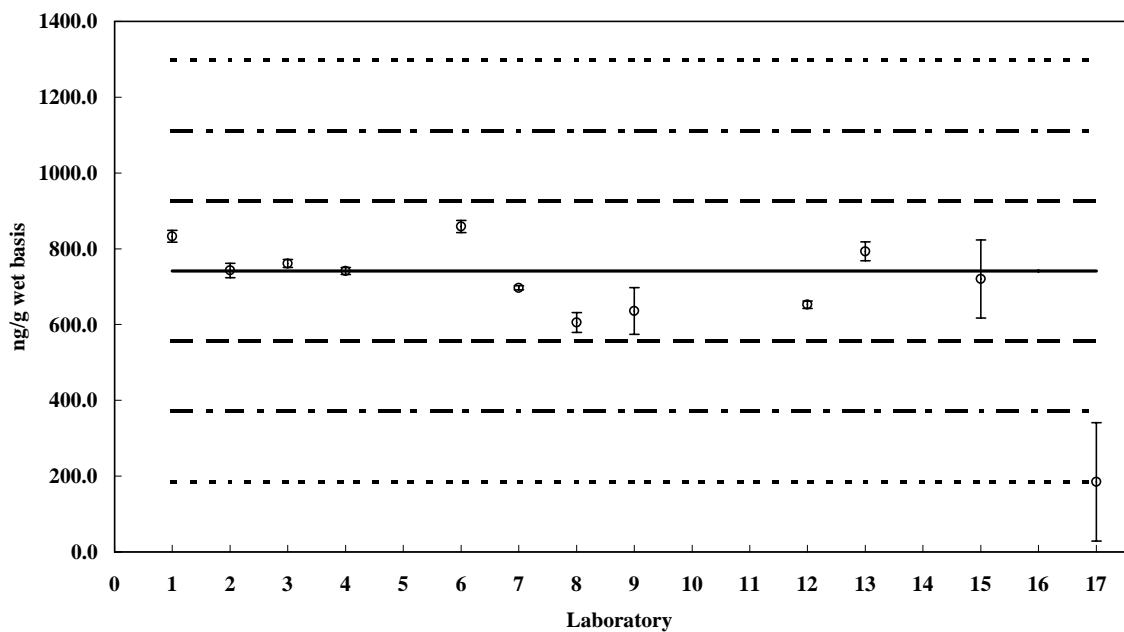**PCB 149**Value = 89.0 \pm 6.9 ng/g (wet basis)

Reported Results: 12

SRM 1945

Certified or Reference Value

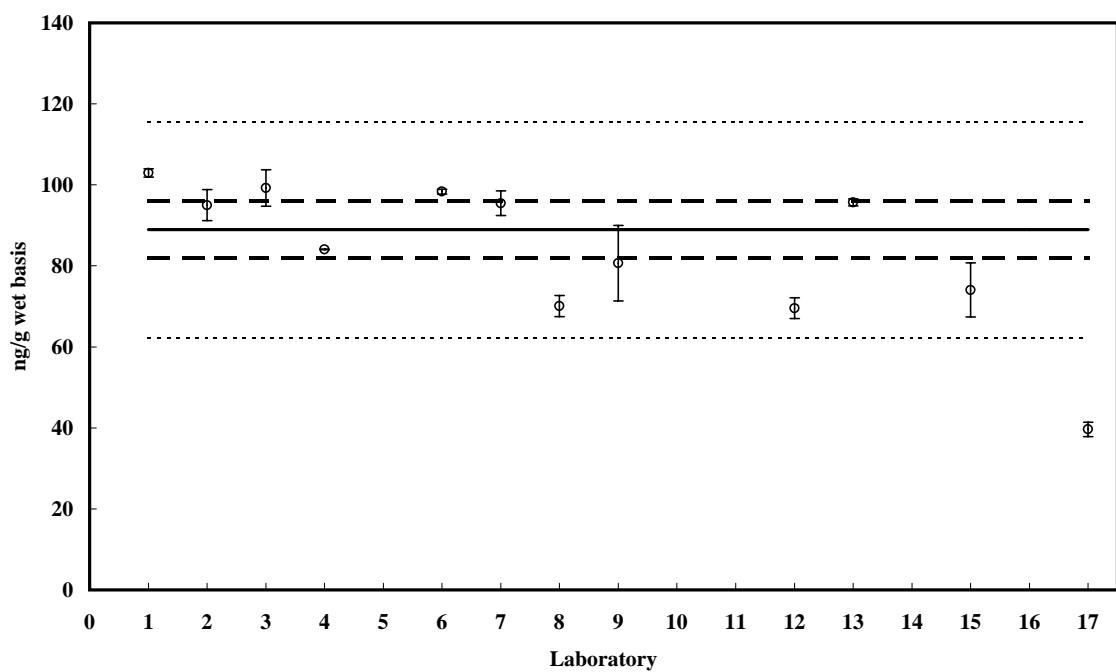 \pm Uncertainty \pm 30 % of Certified or Reference Value


PCB 151

Assigned value = 261 ng/g SD = 32 ng/g 95% CI = \pm 20 ng/g (wet basis)

Reported Results: 10 Quantitative Results: 10

Homogenate VII (Blainville's Beaked Whale)

Assigned Value
 \pm 1 Z
 \pm 2 Z
 \pm 3 Z

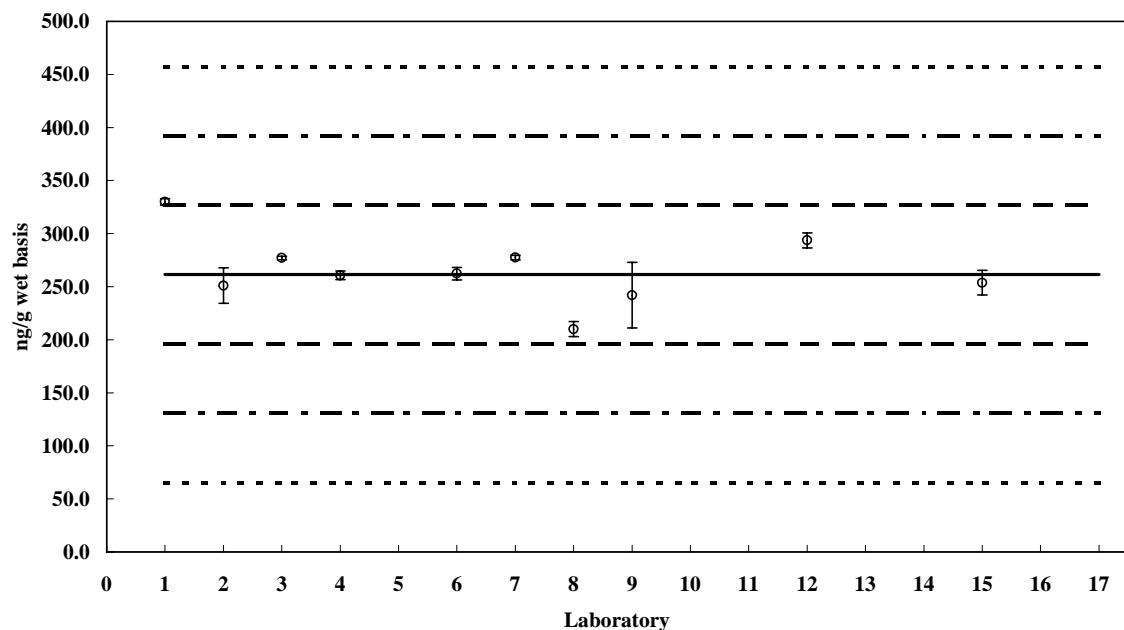

PCB 151

Value = 28.6 \pm 1.3 ng/g (wet basis)


Reported Results: 11

SRM 1945

Certified or Reference Value

\pm Uncertainty

\pm 30 % of Certified or Reference Value

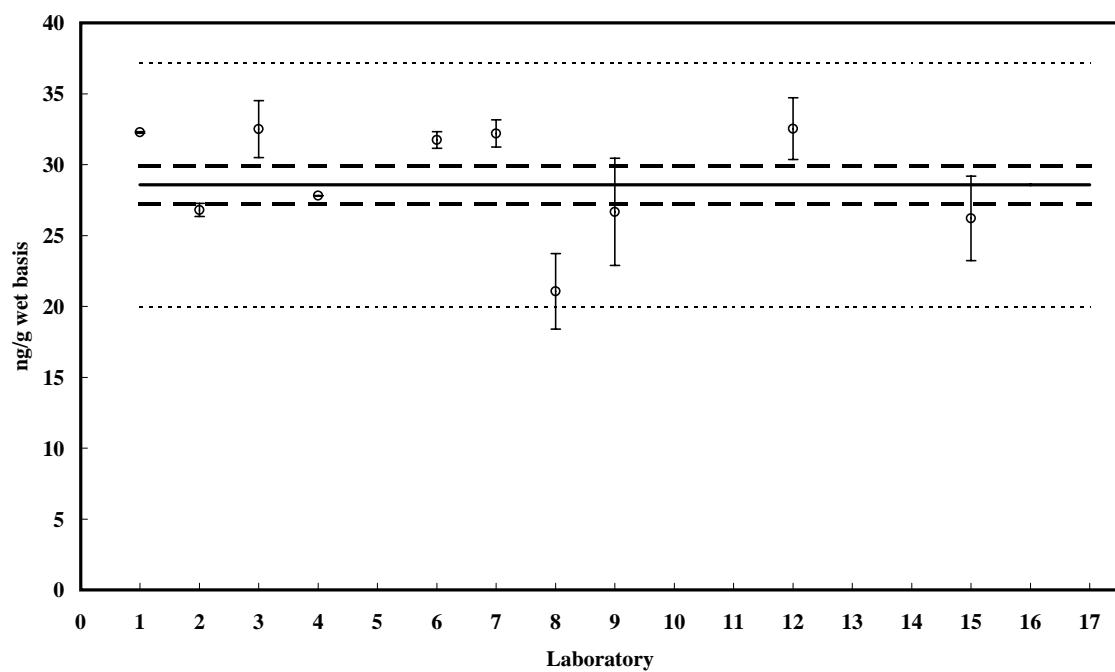


PCB 153

Assigned value = 1831 ng/g SD = 324 ng/g 95% CI = \pm 240 ng/g (wet basis)

Reported Results: 10 Quantitative Results: 7

Homogenate VII (Blainville's Beaked Whale)

____ Assigned Value
- - - \pm 1 Z
- - - \pm 2 Z
- - - - \pm 3 Z

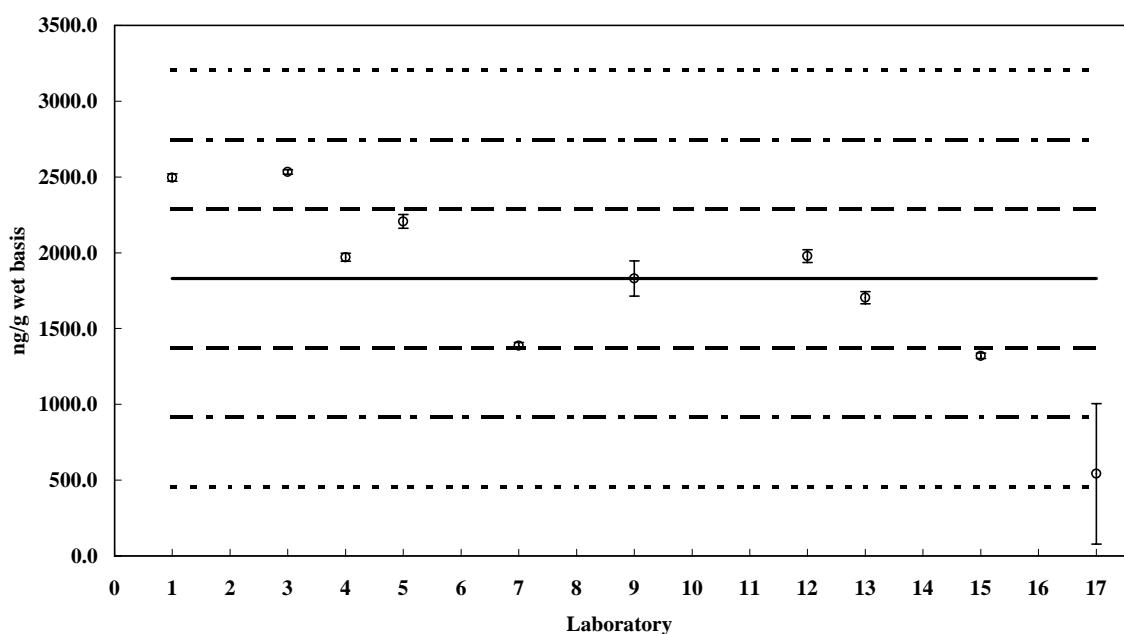

PCB 153

Value = 228 \pm 10 ng/g (wet basis)


Reported Results: 10

SRM 1945

____ Certified or Reference Value

- - - \pm Uncertainty

- - - - \pm 30 % of Certified or Reference Value

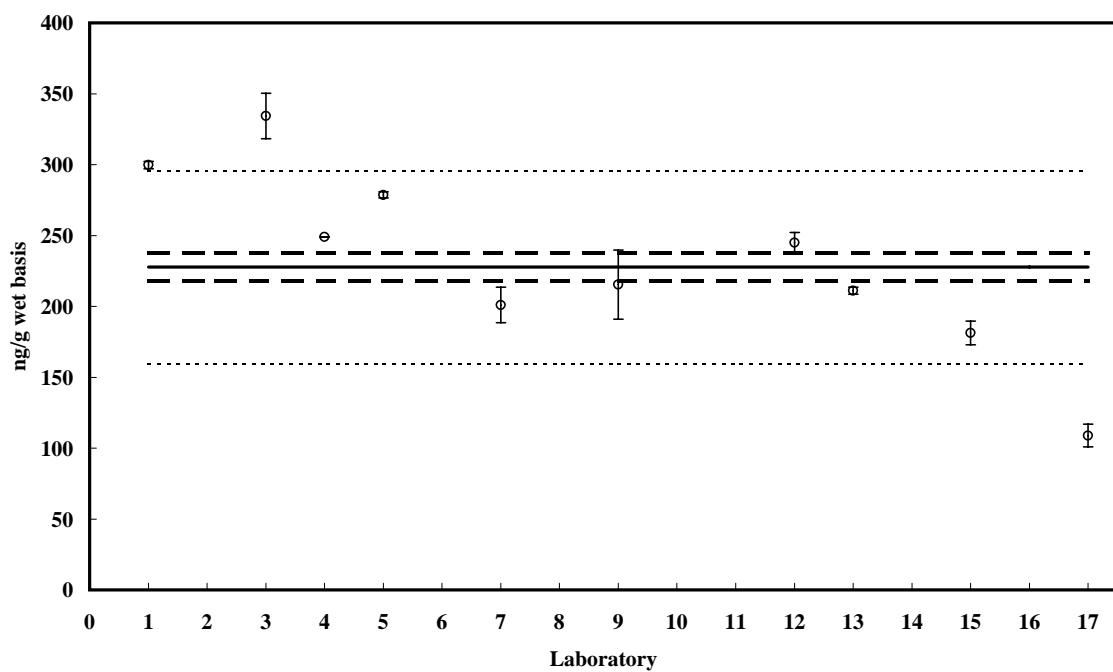


PCB 156

Assigned value = 98.2 ng/g SD = 24 ng/g 95% CI = \pm 15 ng/g (wet basis)

Reported Results: 12 Quantitative Results: 10

Homogenate VII (Blainville's Beaked Whale)

— Assigned Value
- - - \pm 1 Z
- - - \pm 2 Z
- - - - \pm 3 Z

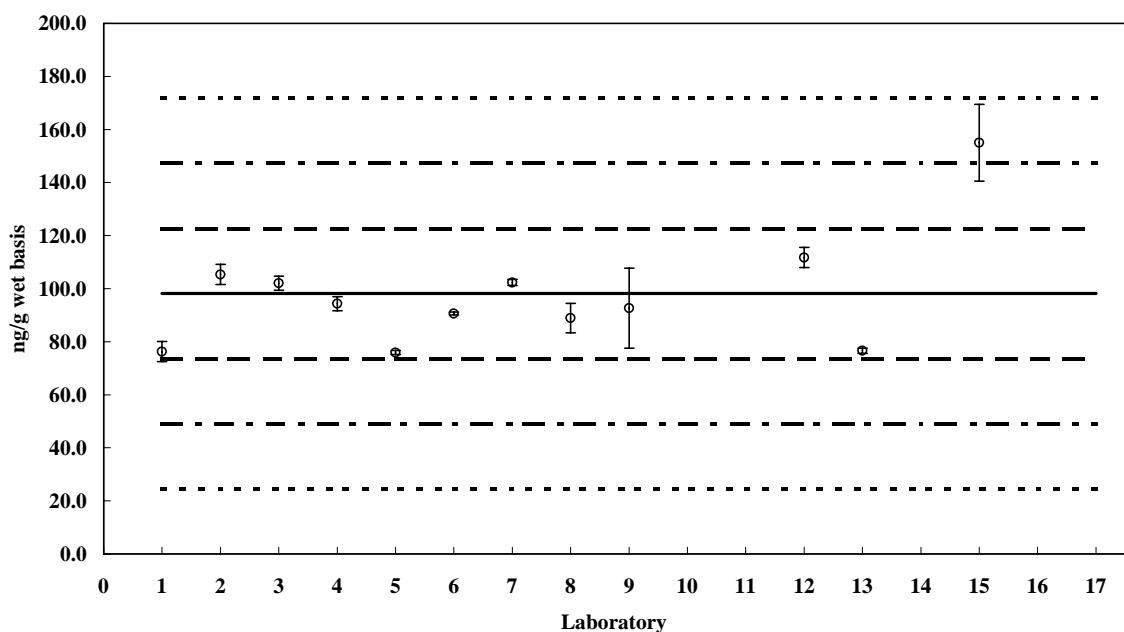


PCB 156

Value = 11.4 \pm 0.95 ng/g (wet basis)

Reported Results: 12

SRM 1945

— Certified or Reference Value
- - - \pm Uncertainty
- - - - \pm 30 % of Ceritifed or Reference Value

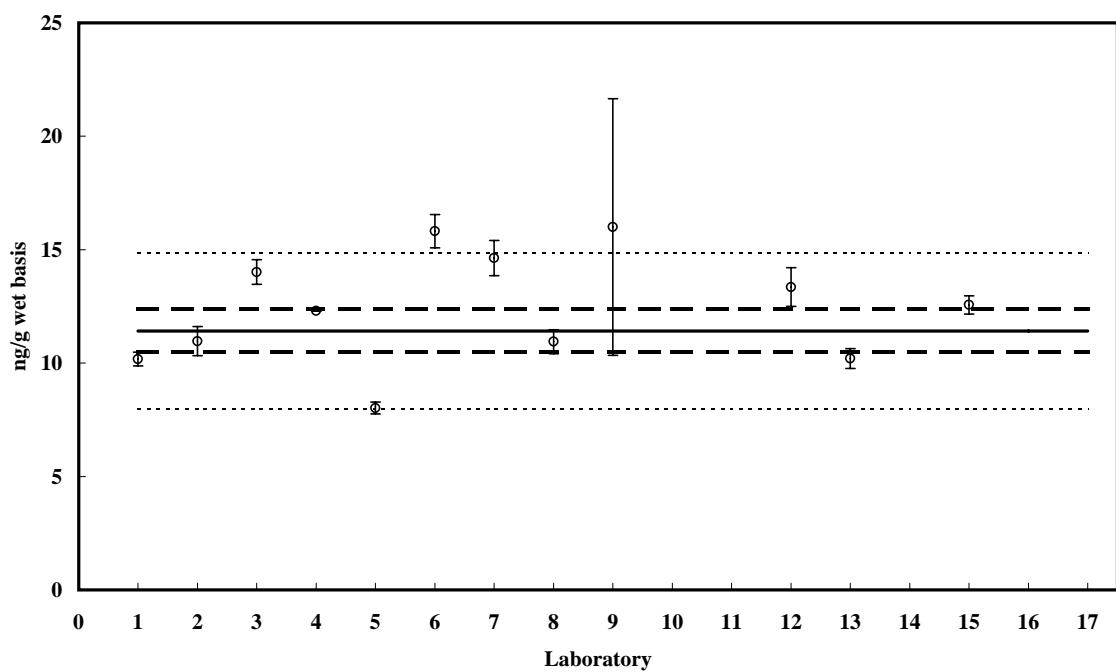


PCB 170 (+190)

Assigned value = 296 ng/g SD = 25 ng/g 95% CI = \pm 16 ng/g (wet basis)

Reported Results: 11 Quantitative Results: 10

Homogenate VII (Blainville's Beaked Whale)

Assigned Value
 \pm 1 Z
 \pm 2 Z
 \pm 3 Z

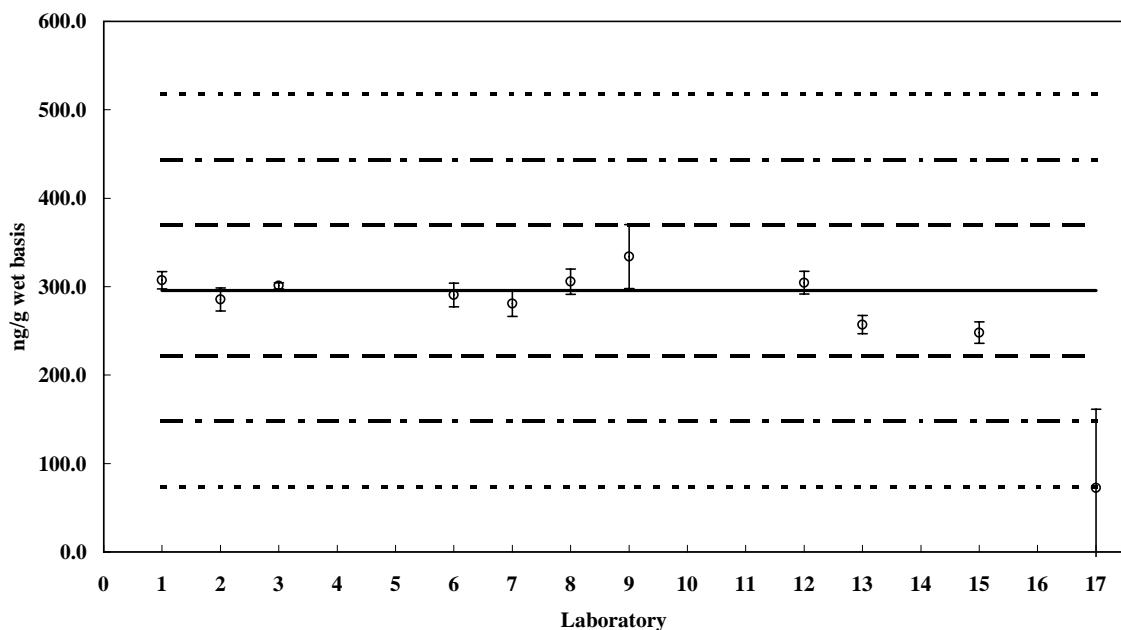

PCB 170 (+190)

Value = 42.6 \pm 2.2 ng/g (wet basis)


Reported Results: 11



SRM 1945



Certified or Reference Value

\pm Uncertainty

\pm 30 % of Certified or Reference Value

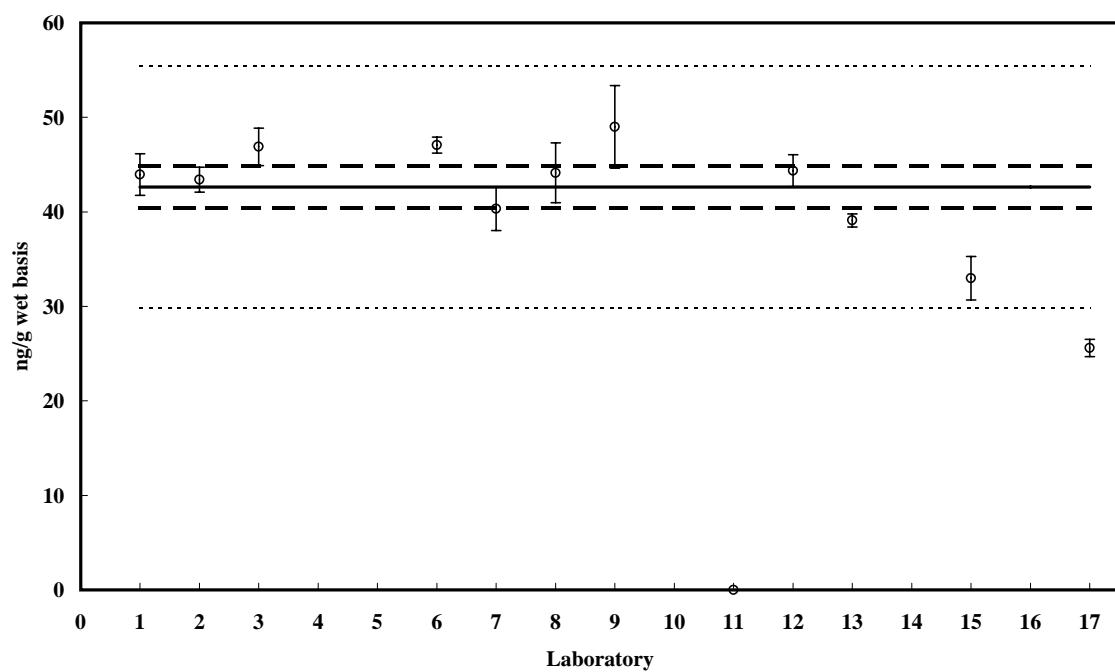

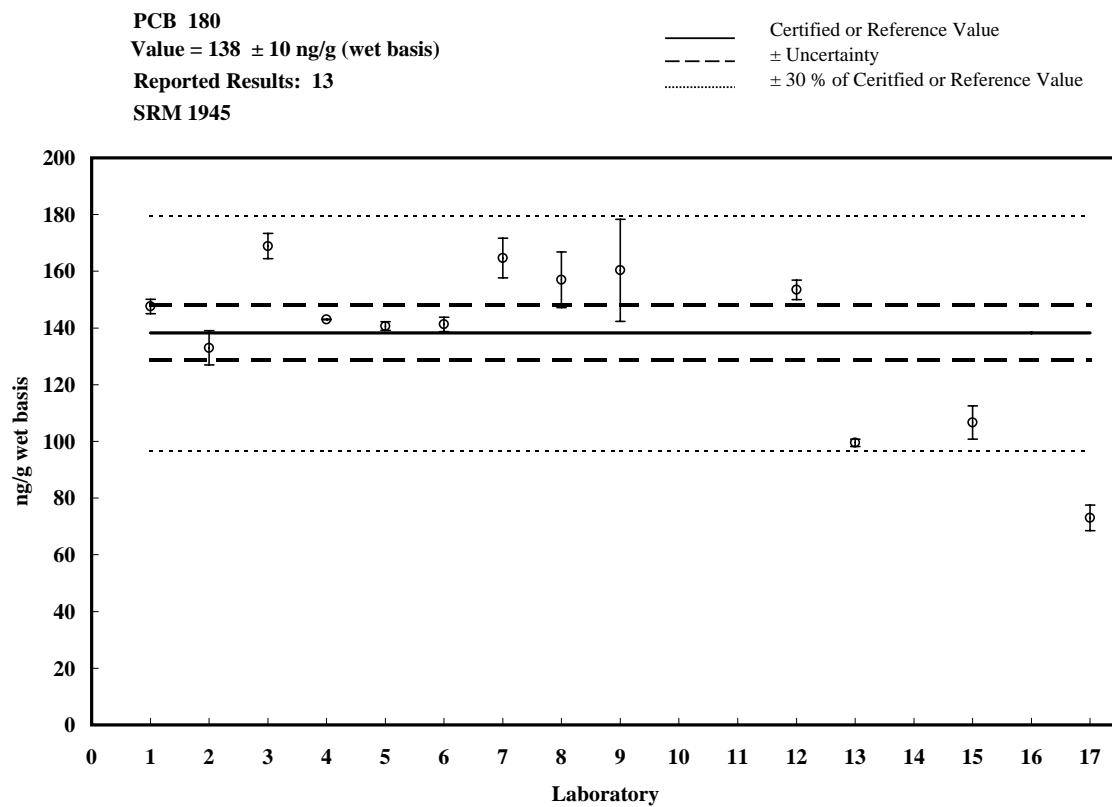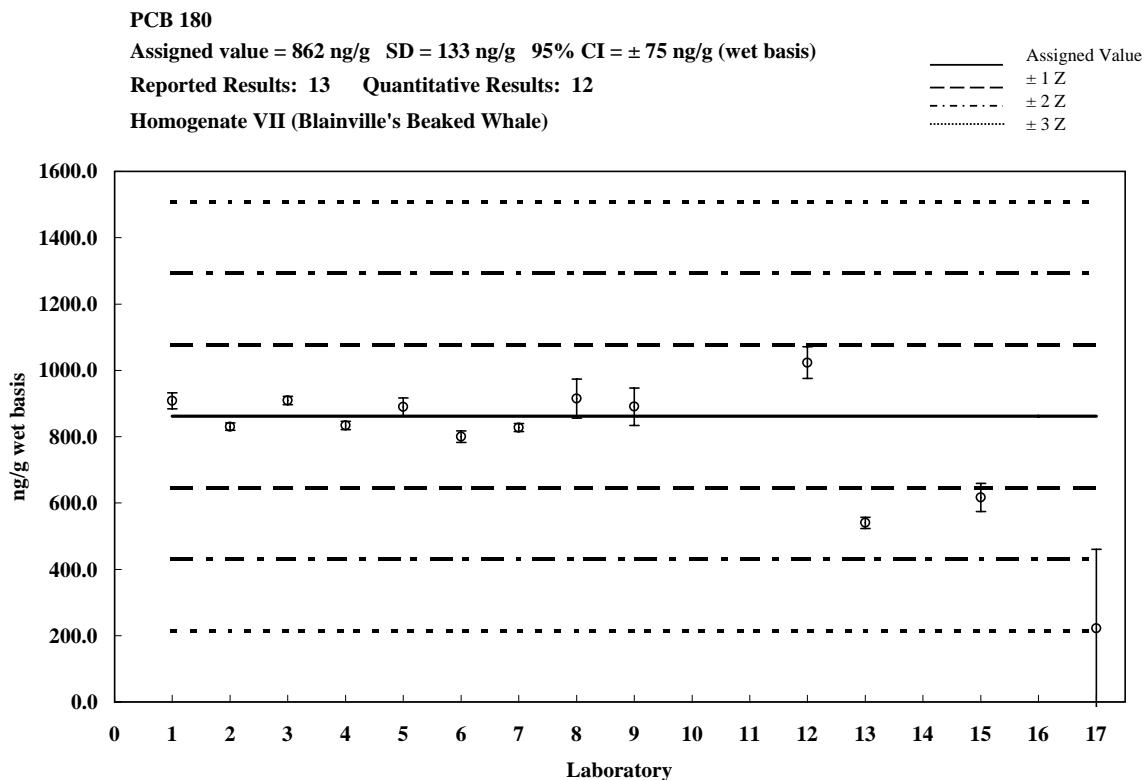

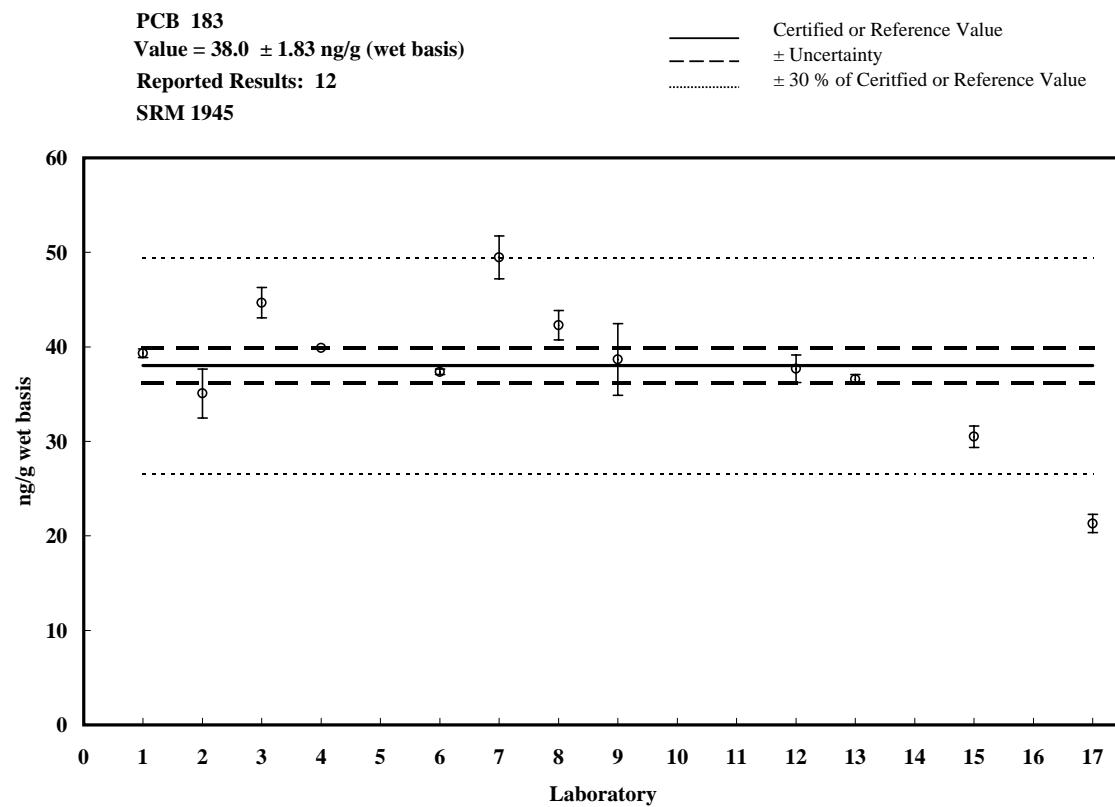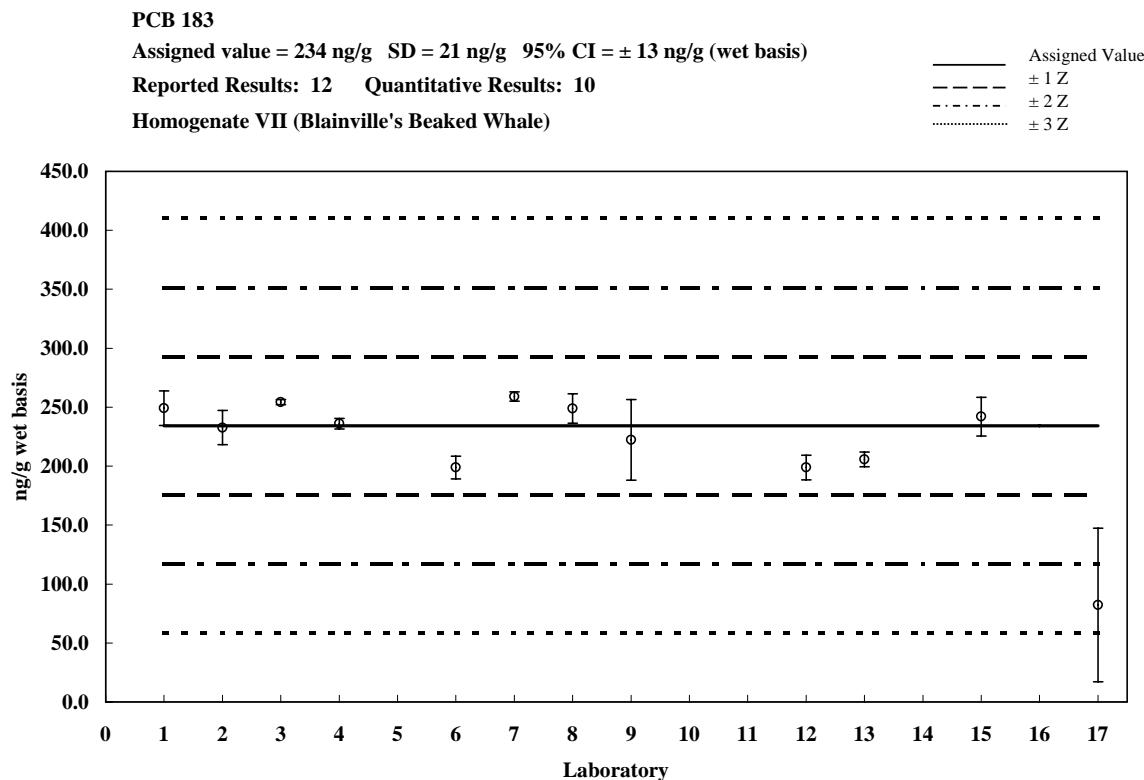


PCB 187

Assigned value = 710 ng/g SD = 116 ng/g 95% CI = \pm 72 ng/g (wet basis)

Reported Results: 12 Quantitative Results: 10

Homogenate VII (Blainville's Beaked Whale)

____ Assigned Value
- - - \pm 1 Z
- - - \pm 2 Z
- - - - \pm 3 Z

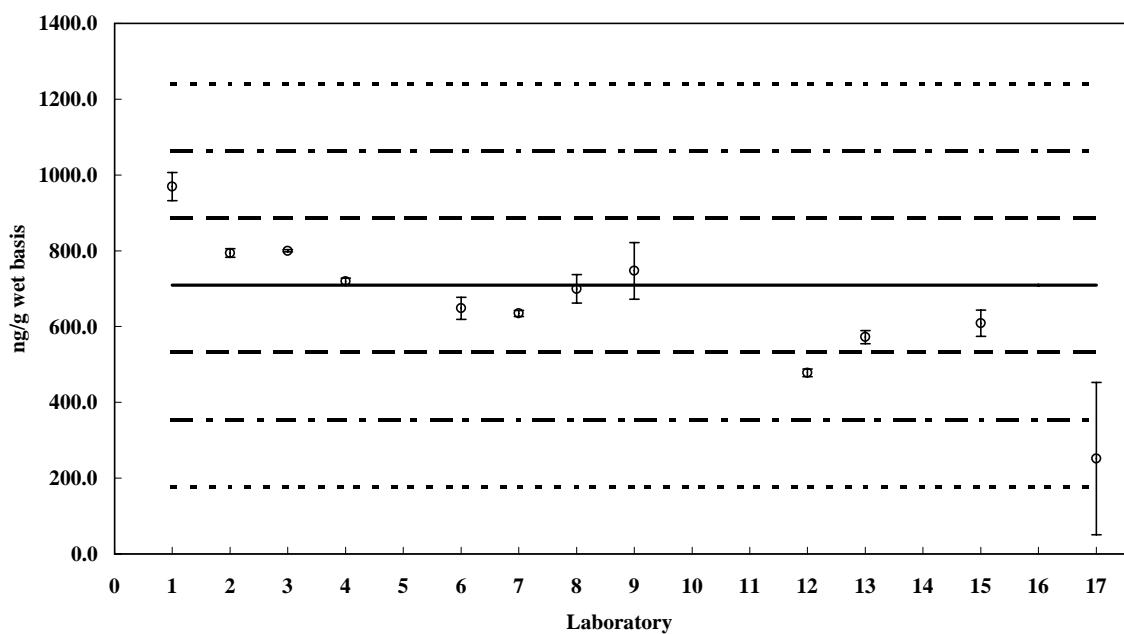

PCB 187

Value = 121 \pm 11 ng/g (wet basis)


Reported Results: 12

SRM 1945

— Certified or Reference Value

- - - \pm Uncertainty

- - - - \pm 30 % of Certified or Reference Value

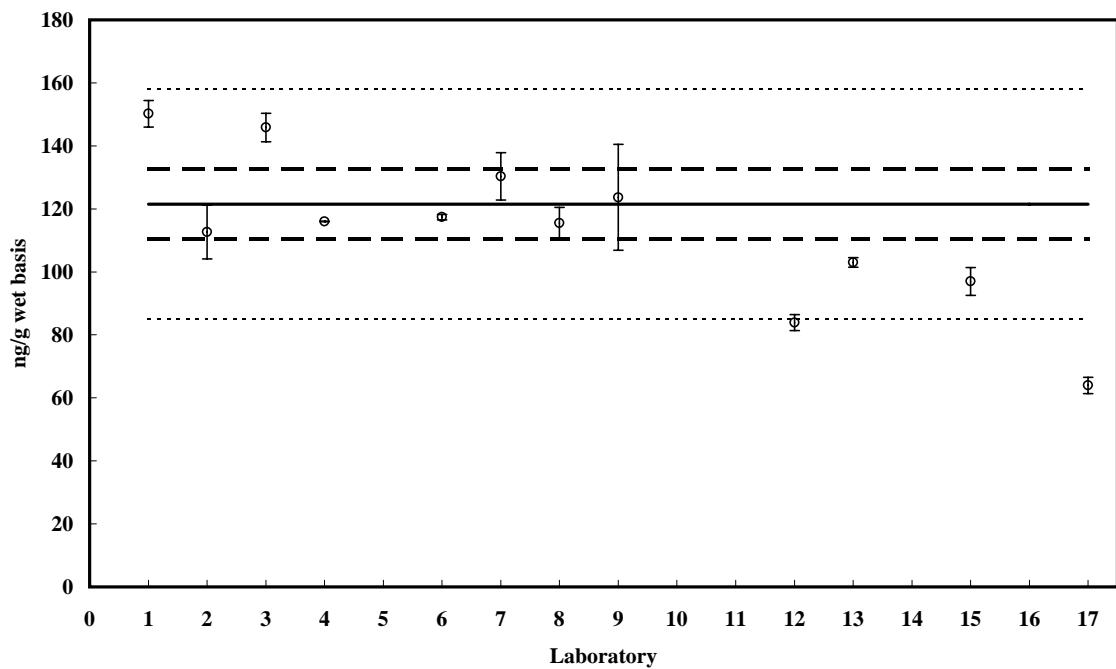


PCB 194

Assigned value = 127 ng/g SD = 22 ng/g 95% CI = \pm 15 ng/g (wet basis)

Reported Results: 12 Quantitative Results: 8

Homogenate VII (Blainville's Beaked Whale)

— Assigned Value
- - - \pm 1 Z
- - - \pm 2 Z
- - - - \pm 3 Z

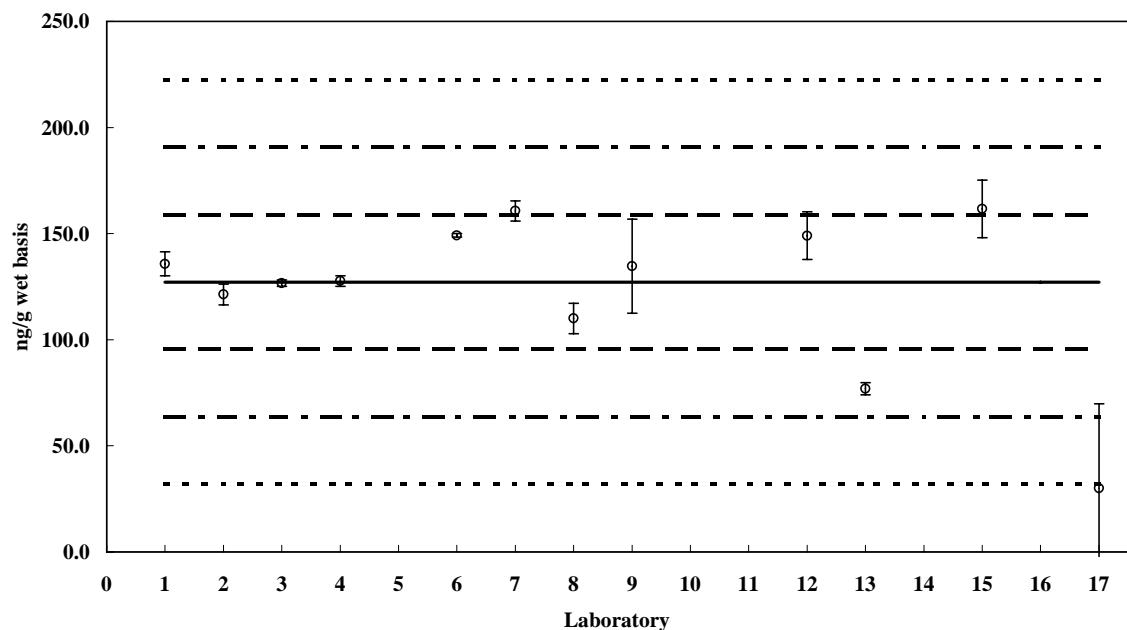

PCB 194

Value = 53.5 \pm 5.2 ng/g (wet basis)


Reported Results: 12

SRM 1945

— Certified or Reference Value

- - - \pm Uncertainty

- - - - \pm 30 % of Certified or Reference Value

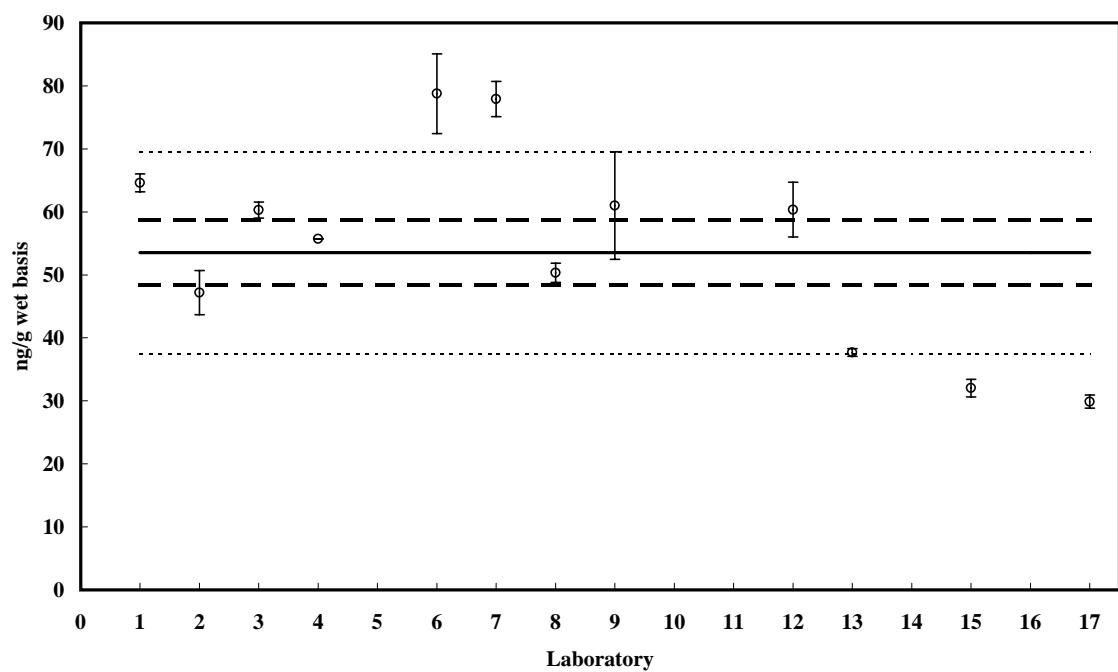


PCB 195

Assigned value = 36.8 ng/g SD = 21 ng/g 95% CI = \pm 14 ng/g (wet basis)

Reported Results: 9 Quantitative Results: 8

Homogenate VII (Blainville's Beaked Whale)

Assigned Value
 \pm 1 Z
 \pm 2 Z
 \pm 3 Z

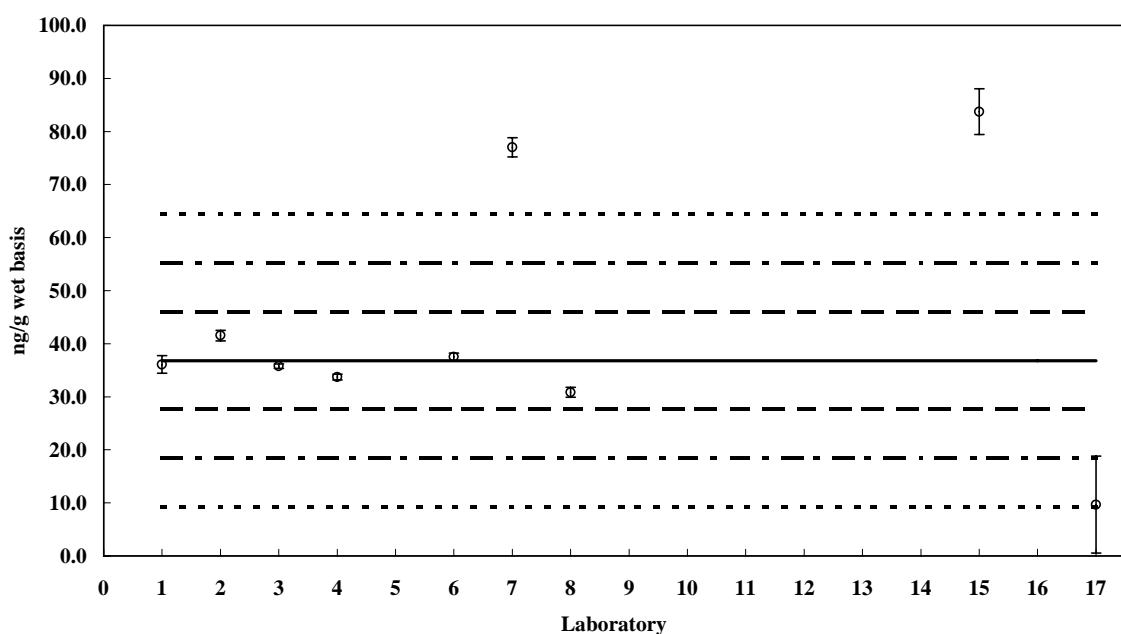

PCB 195

Value = 14.3 \pm 2.2 ng/g (wet basis)


Reported Results: 9

SRM 1945

Certified or Reference Value

\pm Uncertainty

\pm 30 % of Certified or Reference Value

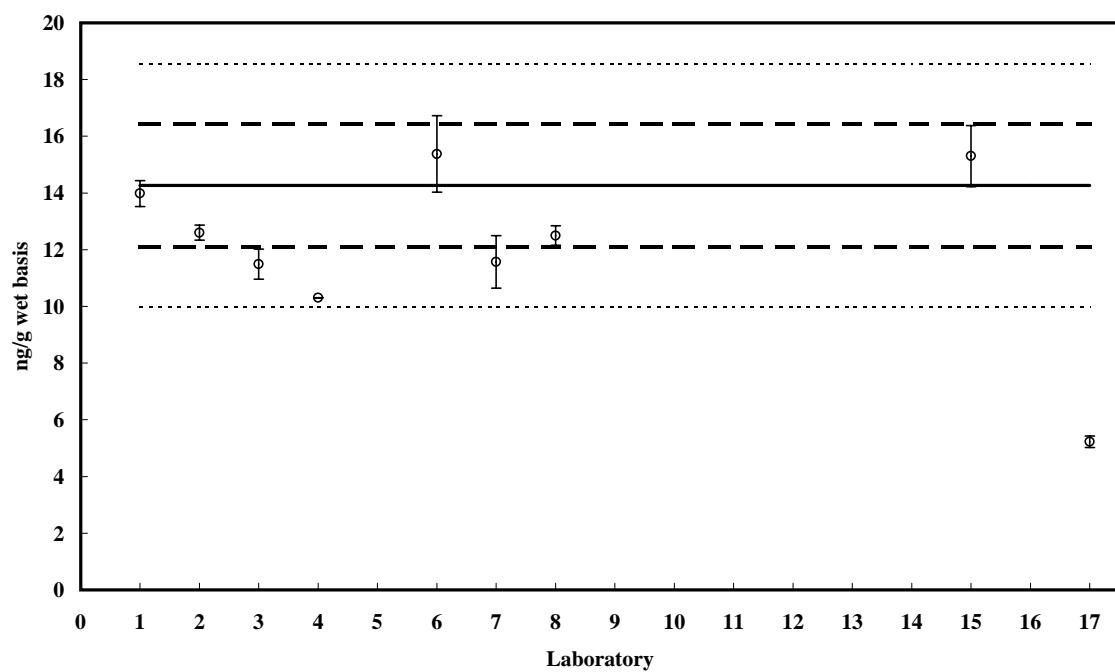


PCB 201

Assigned value = 46.2 ng/g SD = 4.2 ng/g 95% CI = \pm 4.1 ng/g (wet basis)

Reported Results: 9 Quantitative Results: 4

Homogenate VII (Blainville's Beaked Whale)

Assigned Value
 \pm 1 Z
 \pm 2 Z
 \pm 3 Z

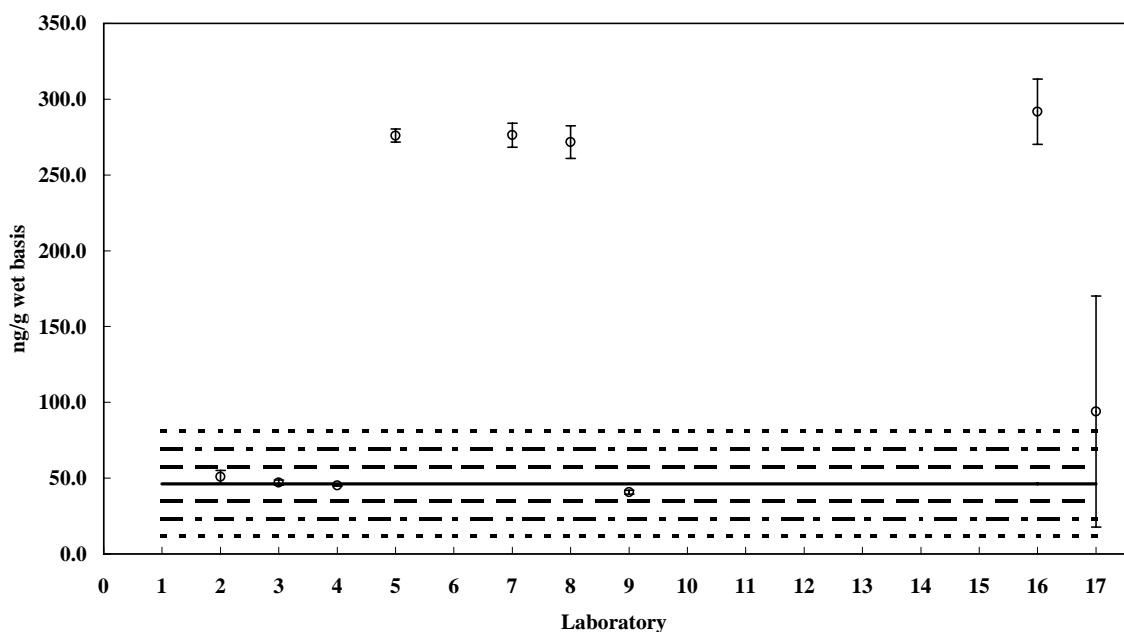

PCB 201

Value = 16.8 \pm 1.3 ng/g (wet basis)


Reported Results: 9

SRM 1945

Certified or Reference Value

\pm Uncertainty

\pm 30 % of Certified or Reference Value

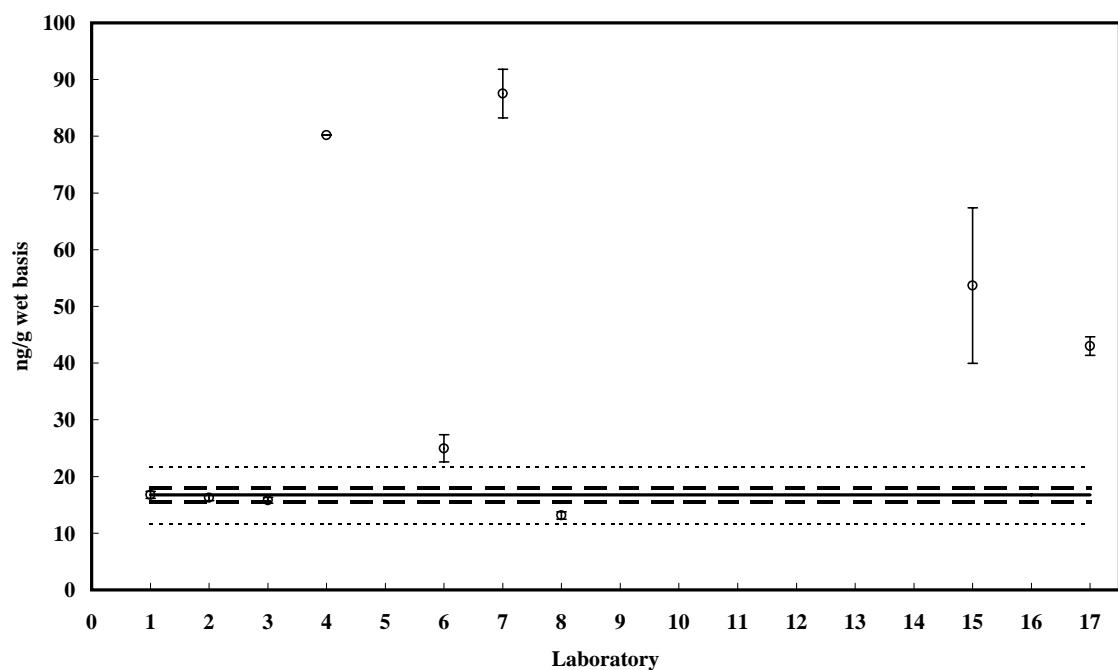


PCB 206

Assigned value = 81.7 ng/g SD = 19 ng/g 95% CI = \pm 13 ng/g (wet basis)

Reported Results: 10 Quantitative Results: 9

Homogenate VII (Blainville's Beaked Whale)

— Assigned Value
- - - \pm 1 Z
- - - \pm 2 Z
- - - - \pm 3 Z

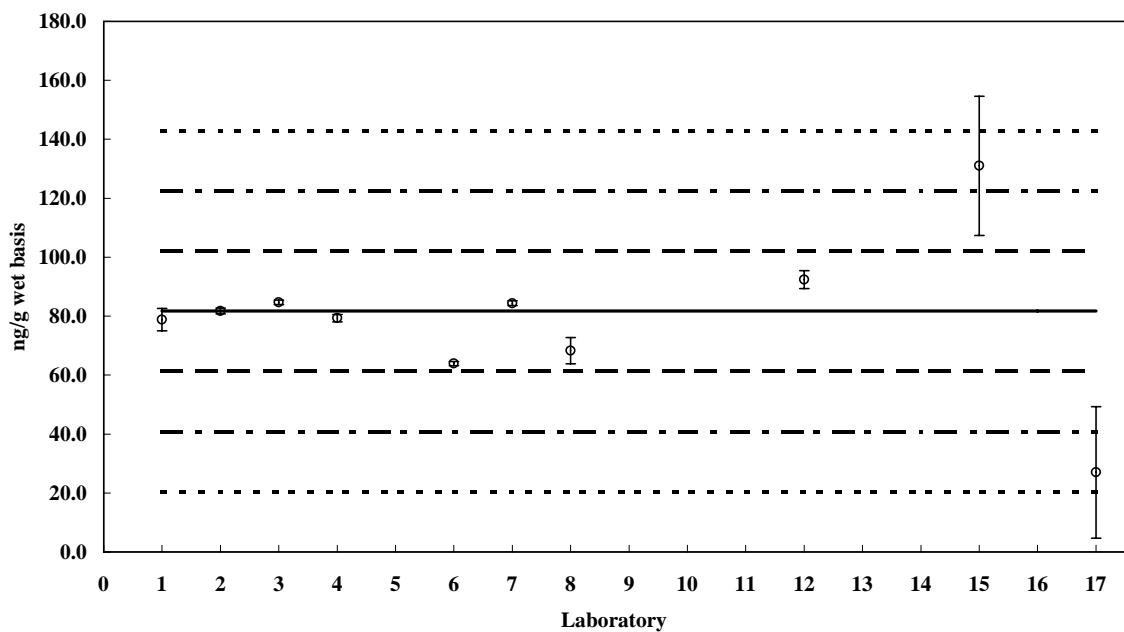

PCB 206

Value = 44.9 \pm 4.2 ng/g (wet basis)


Reported Results: 10

SRM 1945

— Certified or Reference Value

- - - \pm Uncertainty

- - - - \pm 30 % of Ceritifed or Reference Value

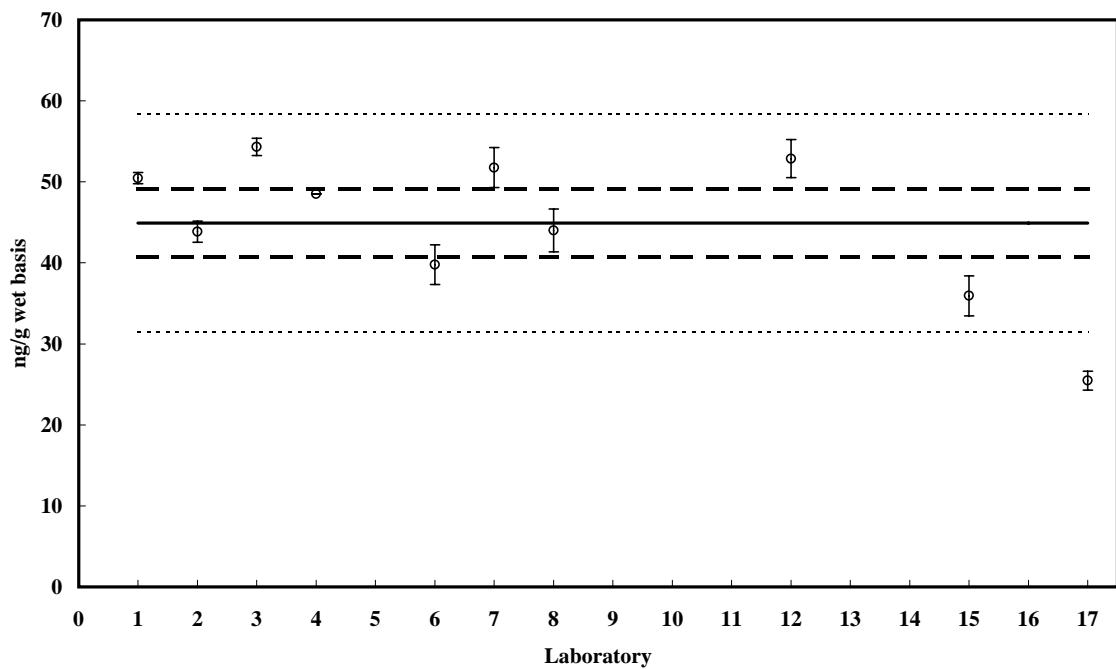


PCB 209

Assigned value = 26.0 ng/g SD = 8.2 ng/g 95% CI = \pm 5.7 ng/g (wet basis)

Reported Results: 10 Quantitative Results: 8

Homogenate VII (Blainville's Beaked Whale)

Assigned Value
 \pm 1 Z
 \pm 2 Z
 \pm 3 Z

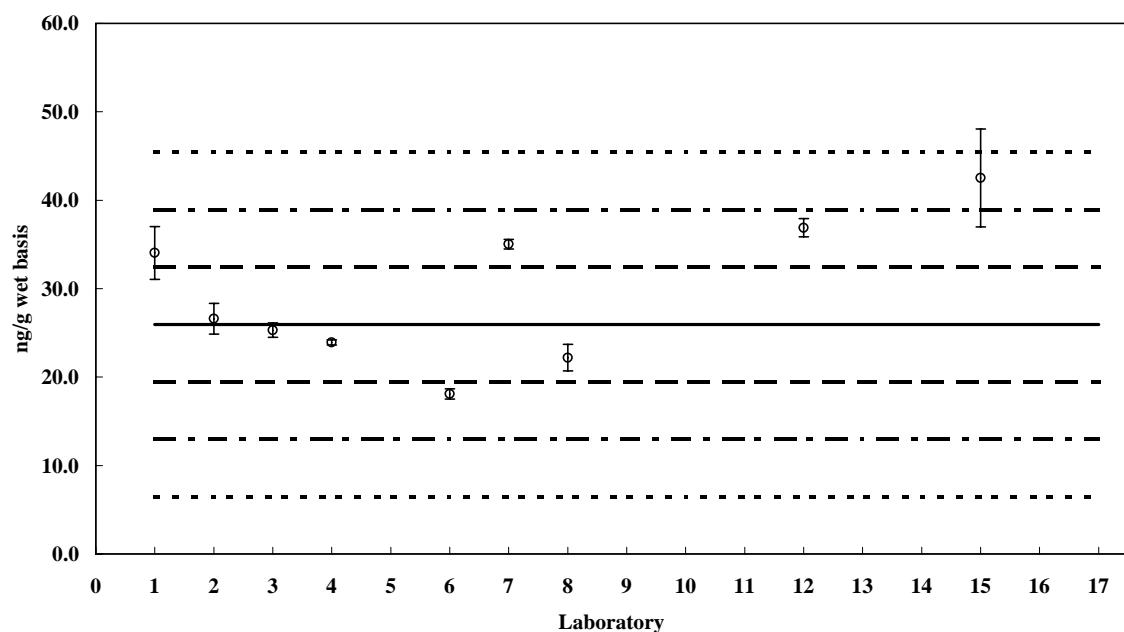

PCB 209

Value = 17.2 \pm 1.9 ng/g (wet basis)


Reported Results: 10

SRM 1945

Certified or Reference Value

\pm Uncertainty

\pm 30 % of Certified or Reference Value

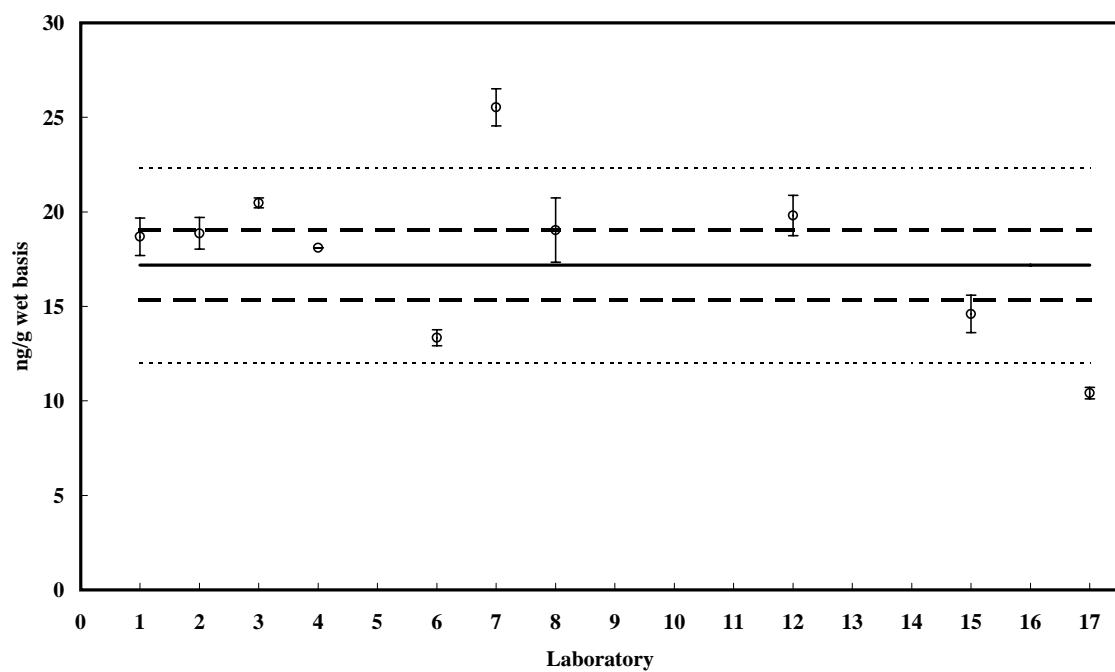


PCB 66

Assigned value = 77.2 ng/g SD = 61 ng/g 95% CI = \pm 40 ng/g (wet basis)

Reported Results: 10 Quantitative Results: 9

Homogenate VII (Blainville's Beaked Whale)

— Assigned Value
- - - \pm 1 Z
- - - - \pm 2 Z
- - - - - \pm 3 Z

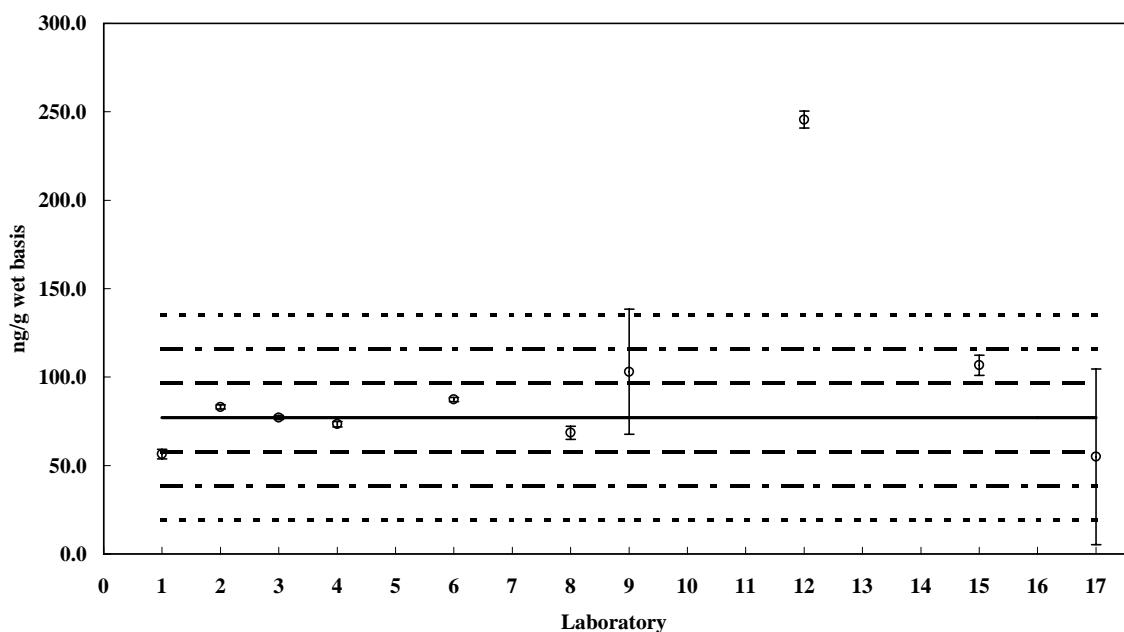

PCB 66

Value = 22.4 \pm 0.5 ng/g (wet basis)


Reported Results: 10



SRM 1945

— Certified or Reference Value

- - - \pm Uncertainty

..... \pm 30 % of Ceritifed or Reference Value

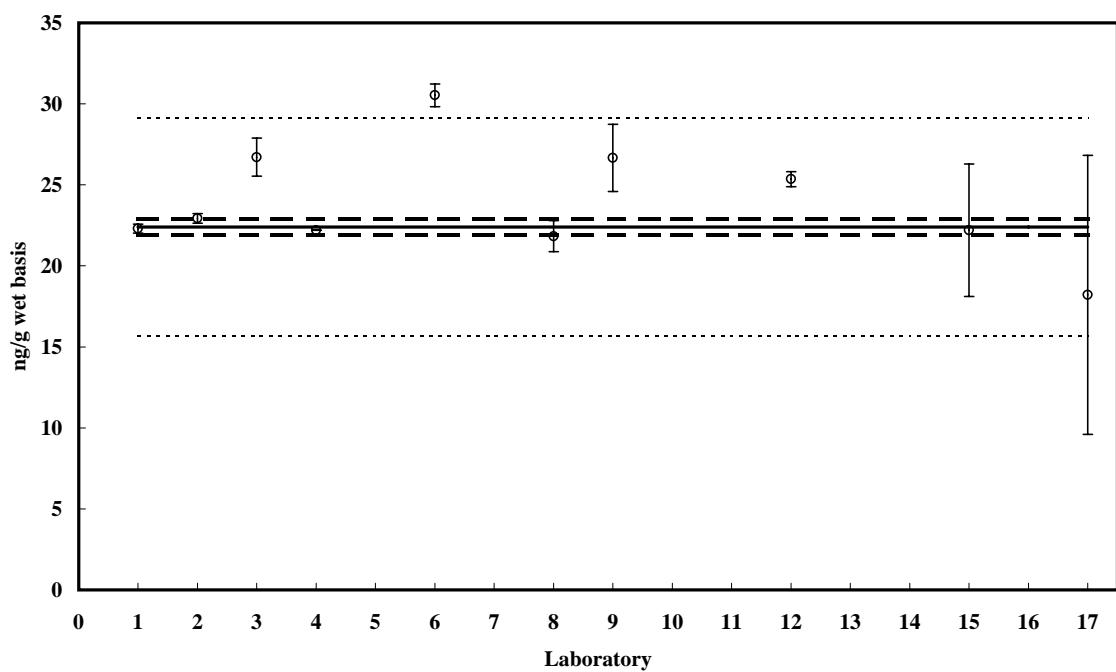

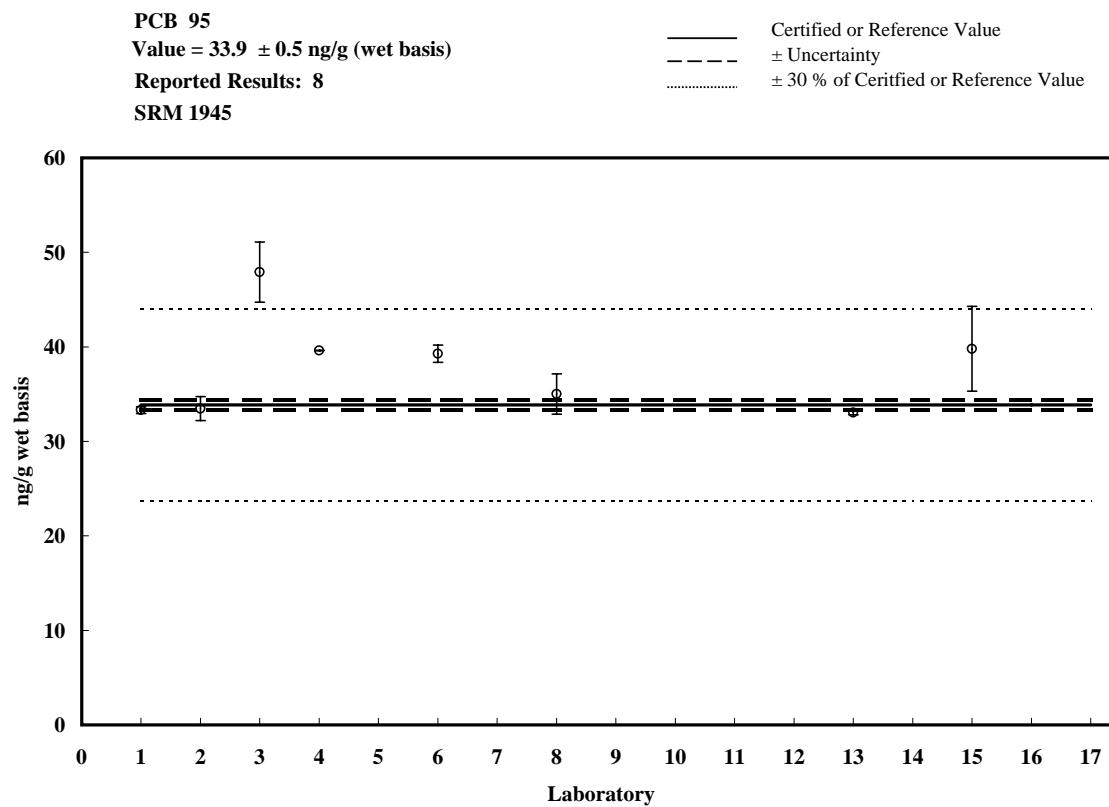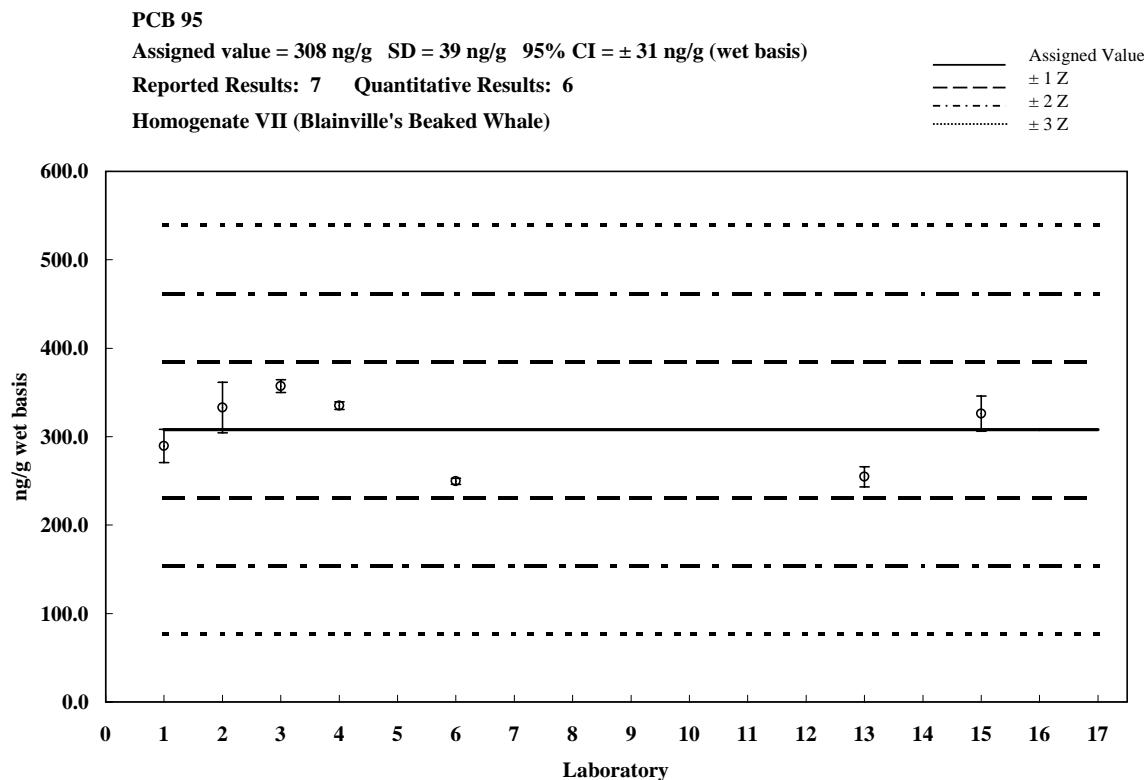


Appendix C

Graphical results of pesticide and lipid data reported by all laboratories. The Z-scores for Homogenate VII represent 25 % of the assigned value so that z = +1 is the assigned value plus 25 %, z = -1 is the assigned value minus 25 % and so forth. Error bars are \pm 1 standard deviation.


2,4'-DDT
Assigned value = 428 ng/g SD = 304 ng/g 95% CI = \pm 243 ng/g (wet basis)
Reported Results: 12 Quantitative Results: 6
Homogenate VII (Blainville's Beaked Whale)



Assigned Value
 \pm 1 Z
 \pm 2 Z
 \pm 3 Z

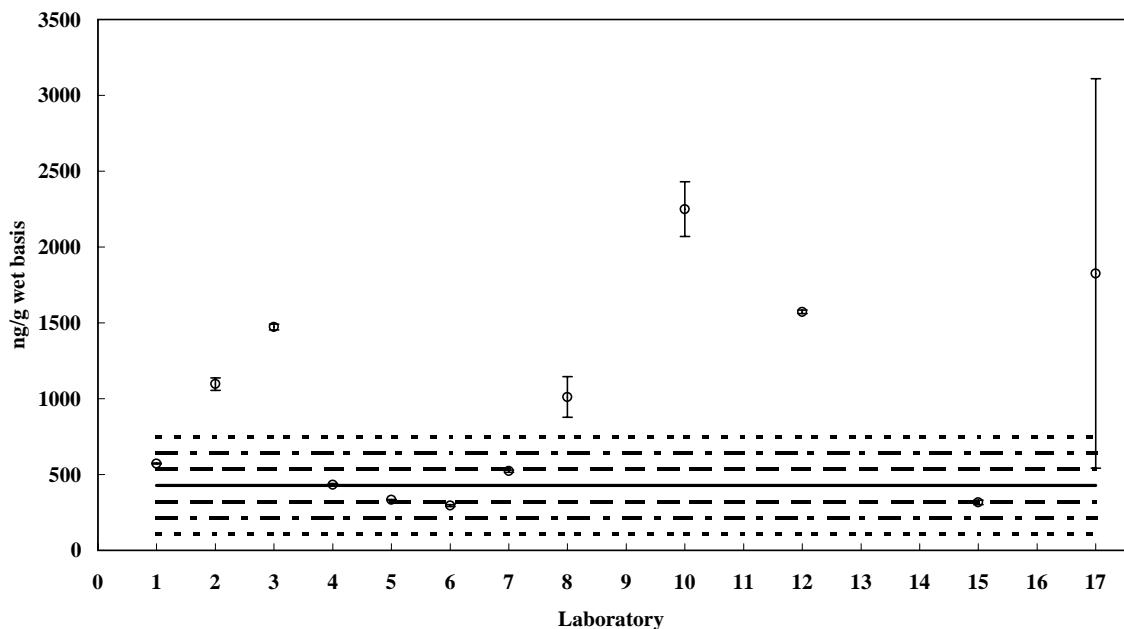




2,4'-DDT
Value = 91.0 \pm 13 ng/g (wet basis)
Reported Results: 12
SRM 1945

Certified or Reference Value
 \pm Uncertainty
 \pm 30 % of Certified or Reference Value

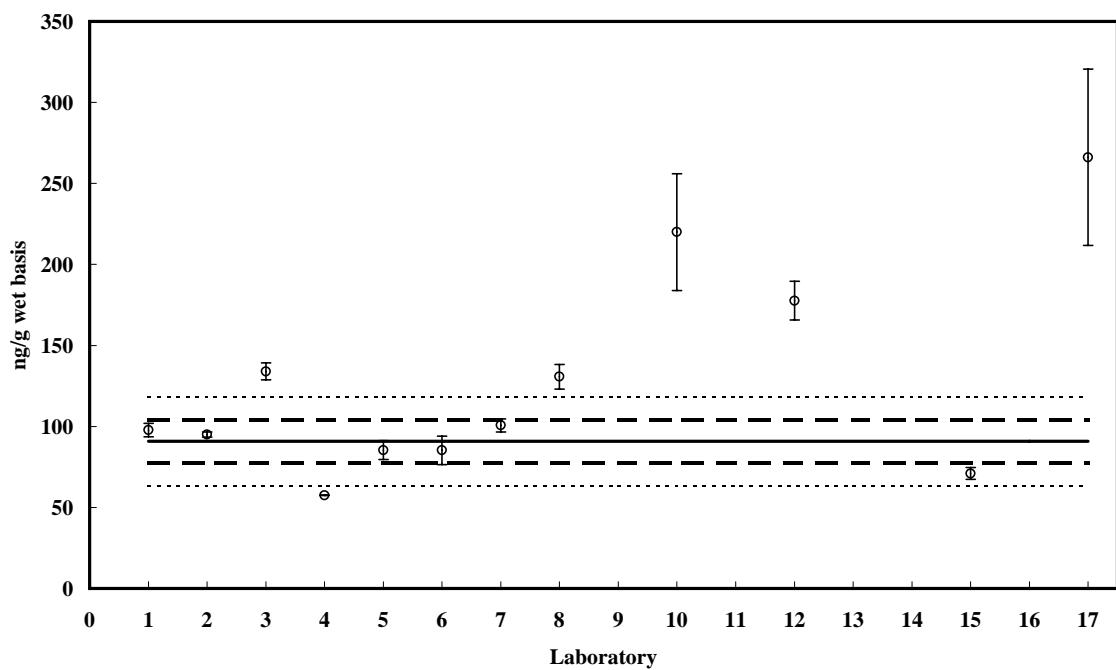

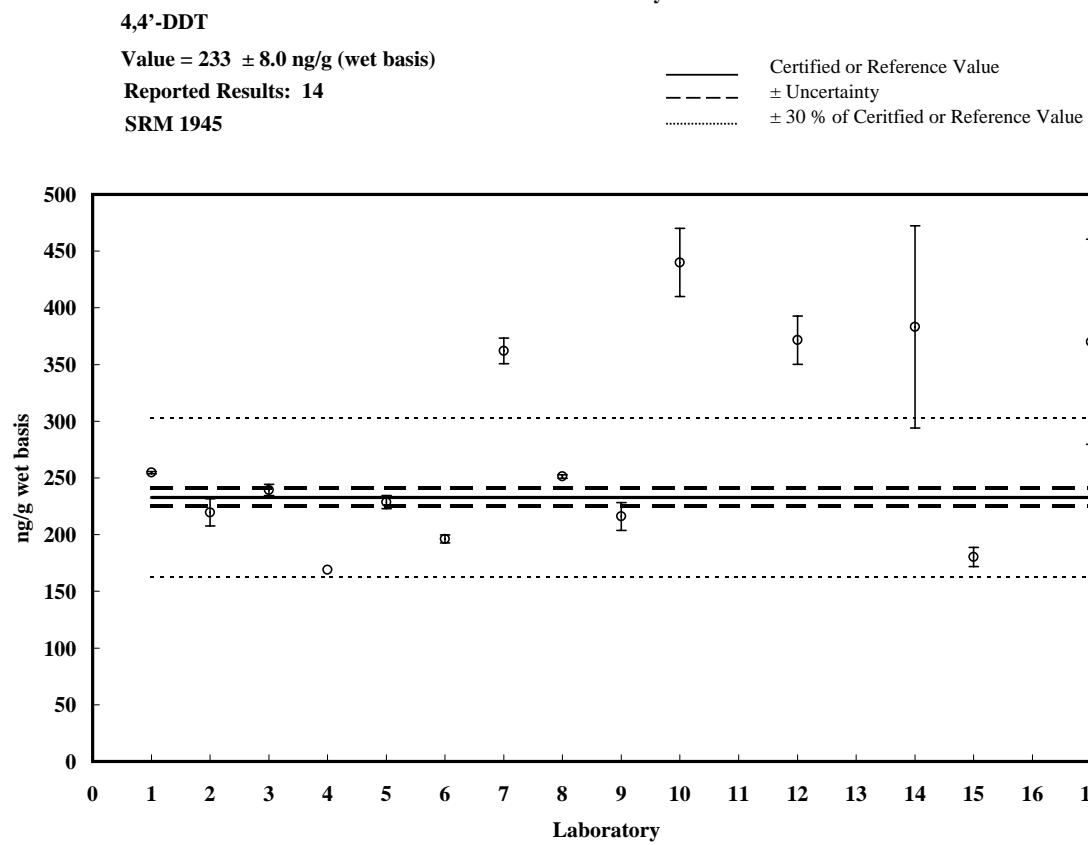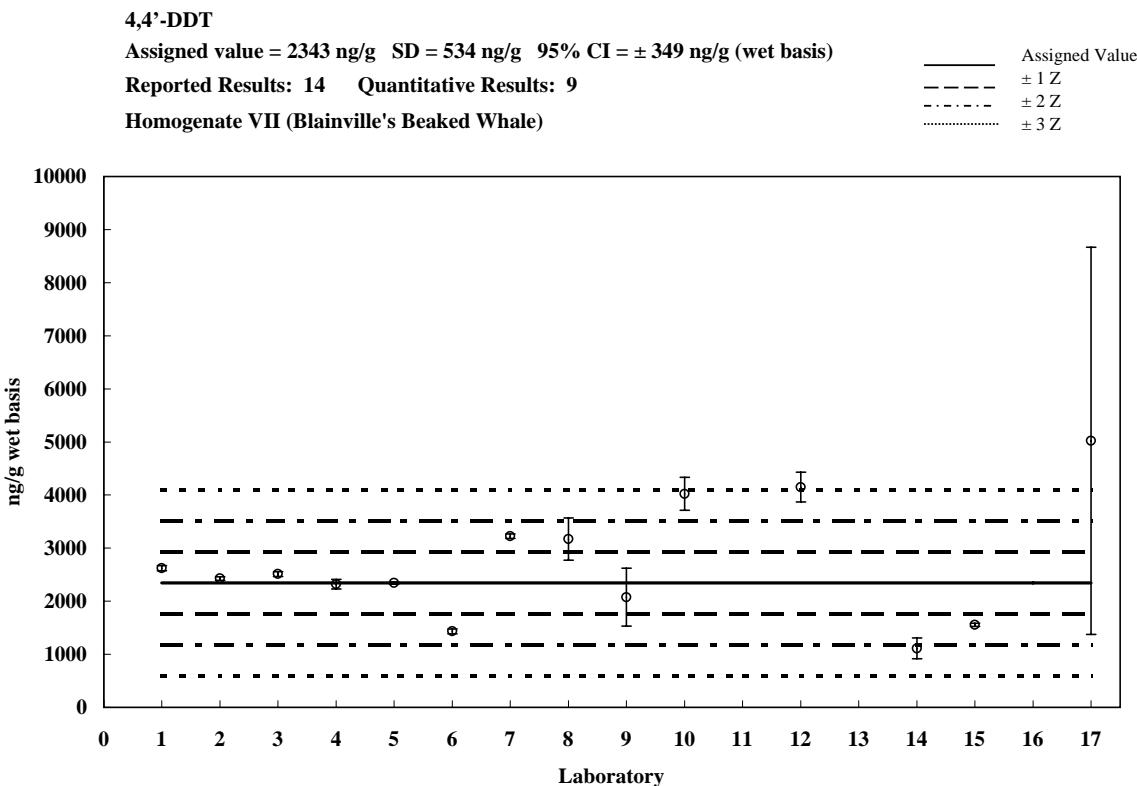


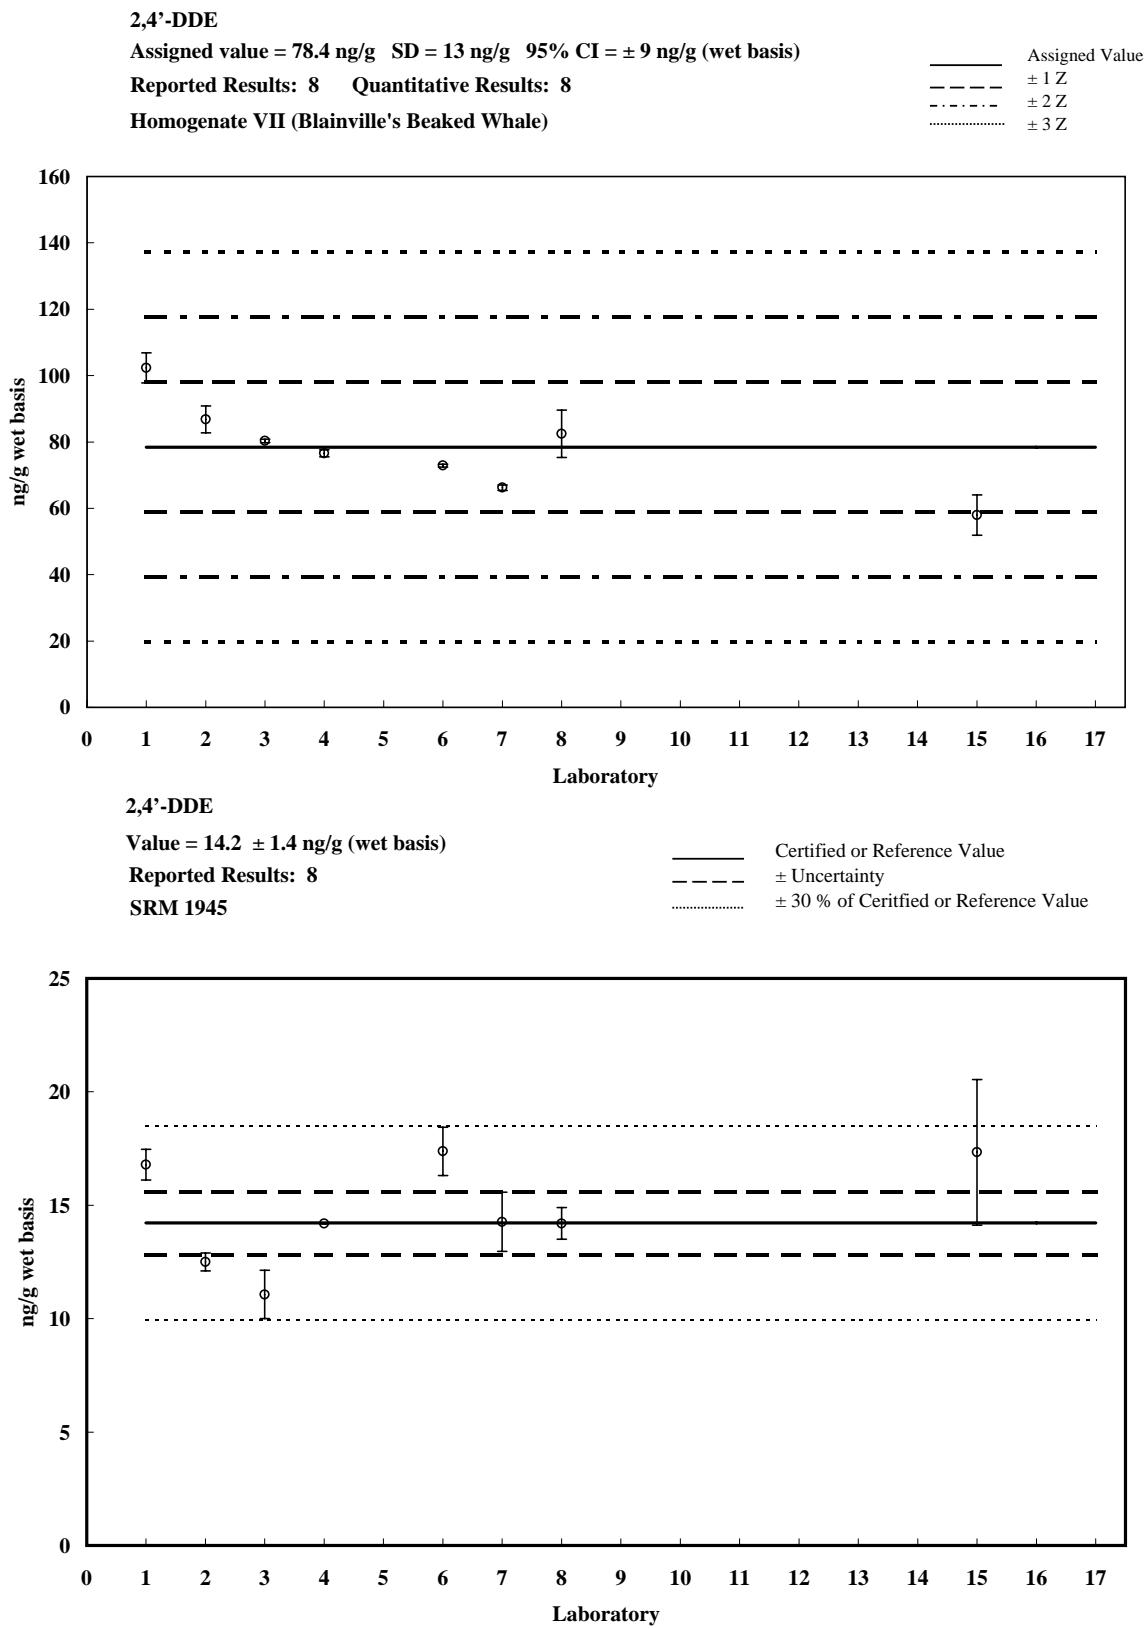

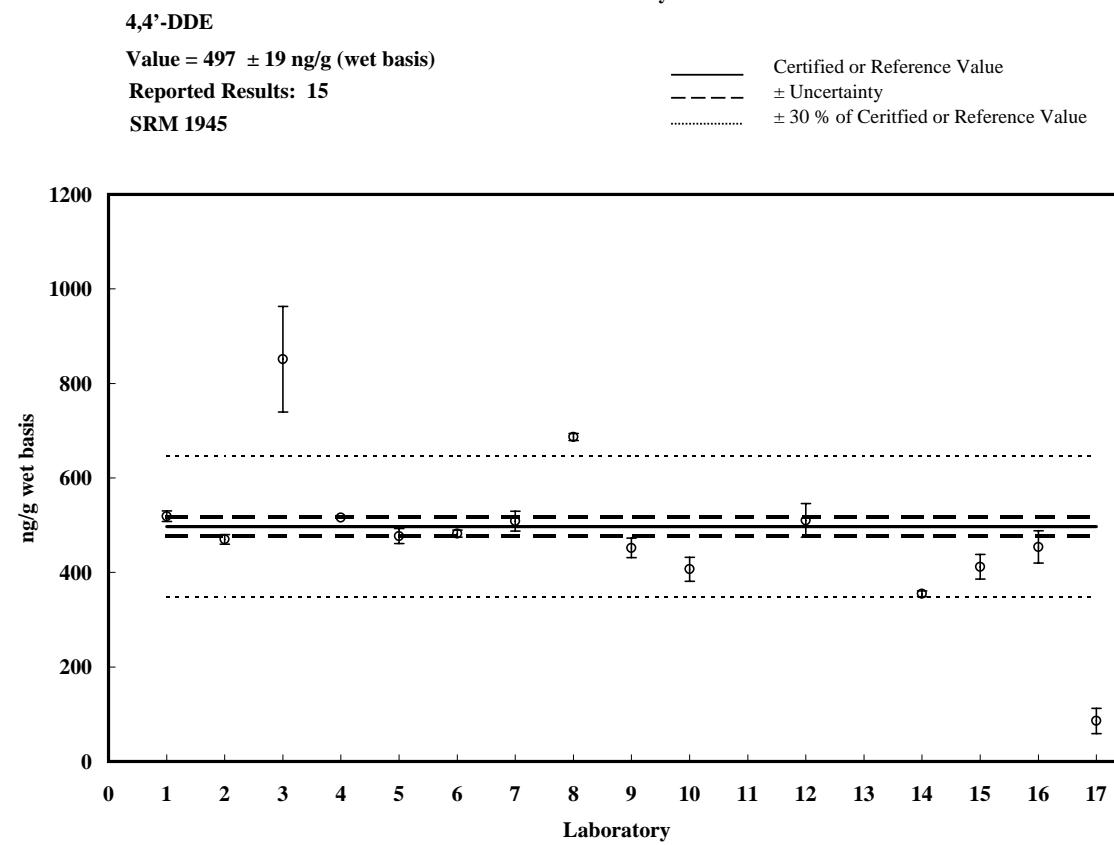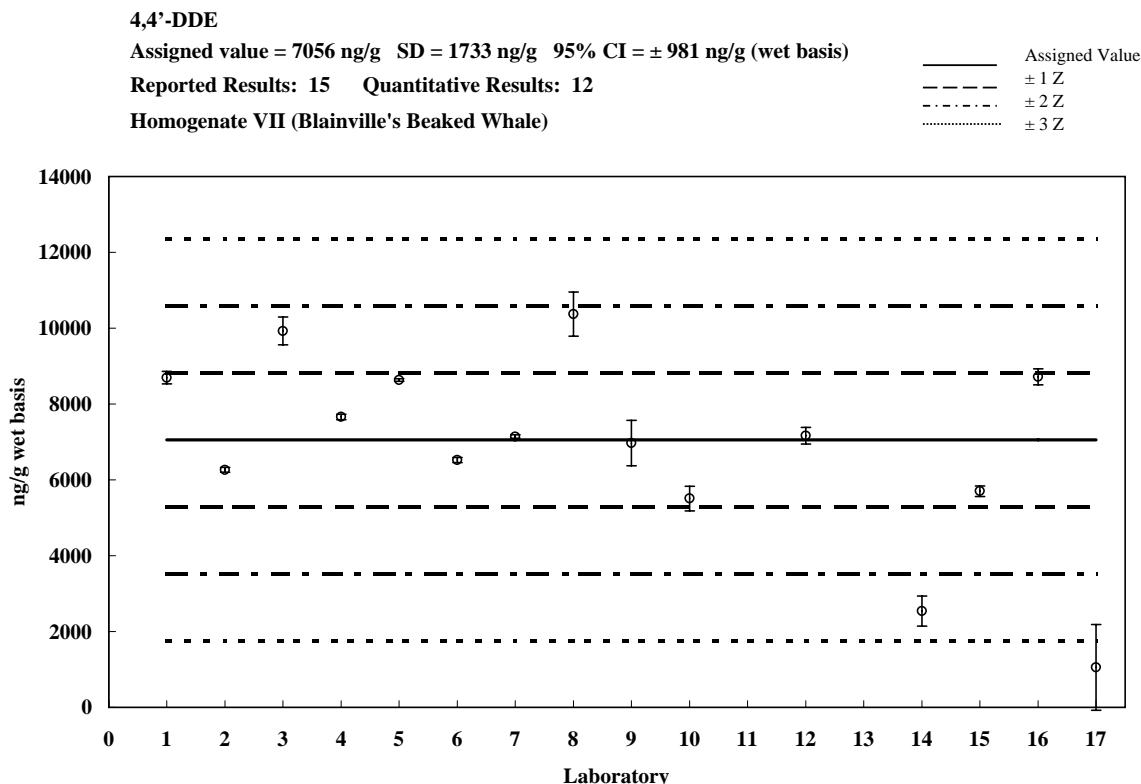


2,4'-DDD
Assigned value = 97 ng/g SD = 43 ng/g 95% CI = \pm 28 ng/g (wet basis)
Reported Results: 11 Quantitative Results: 9
Homogenate VII (Blainville's Beaked Whale)



Assigned Value
 \pm 1 Z
 \pm 2 Z
 \pm 3 Z


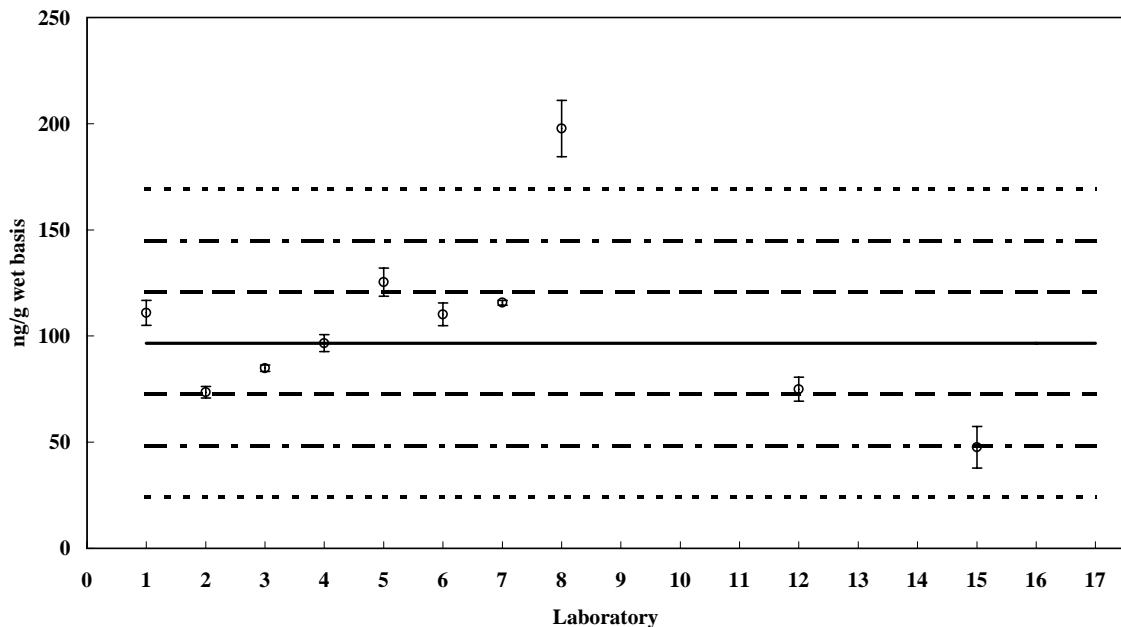


2,4'-DDD
Value = 19.5 \pm 1.2 ng/g (wet basis)
Reported Results: 11
SRM 1945

Certified or Reference Value
 \pm Uncertainty
 \pm 30 % of Certified or Reference Value

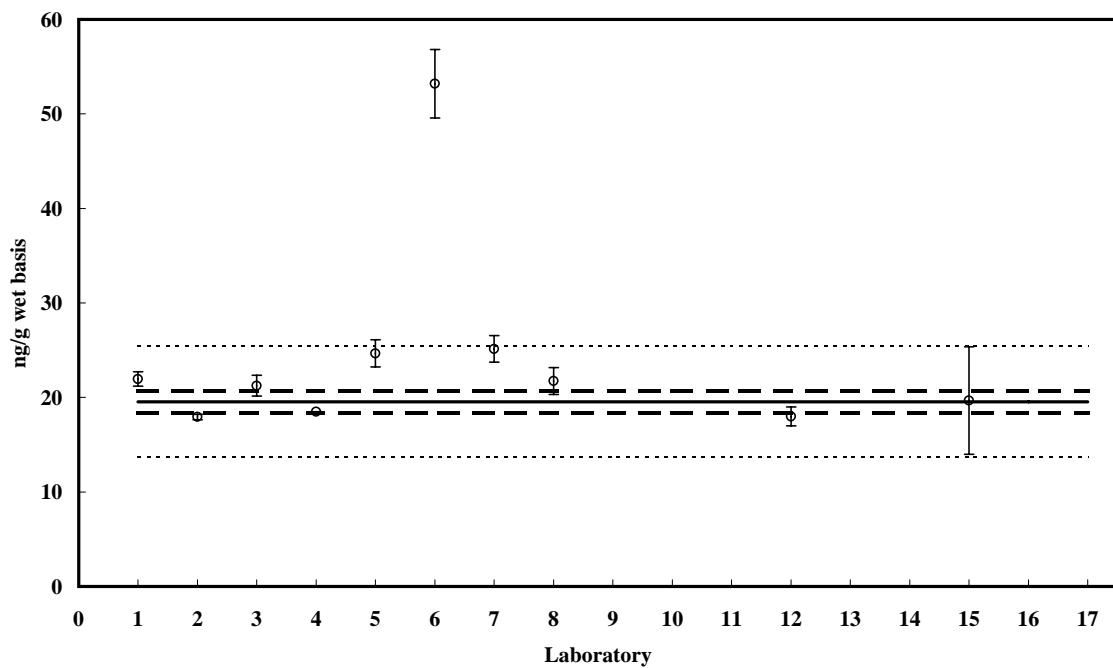

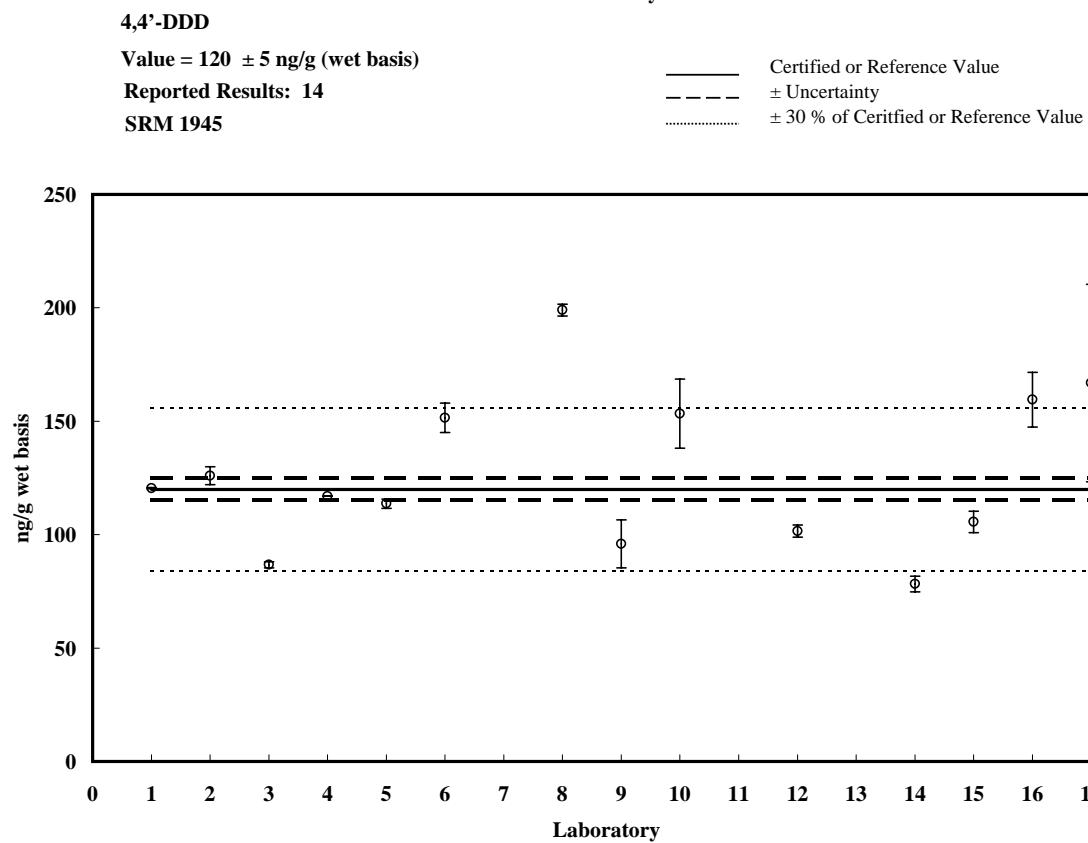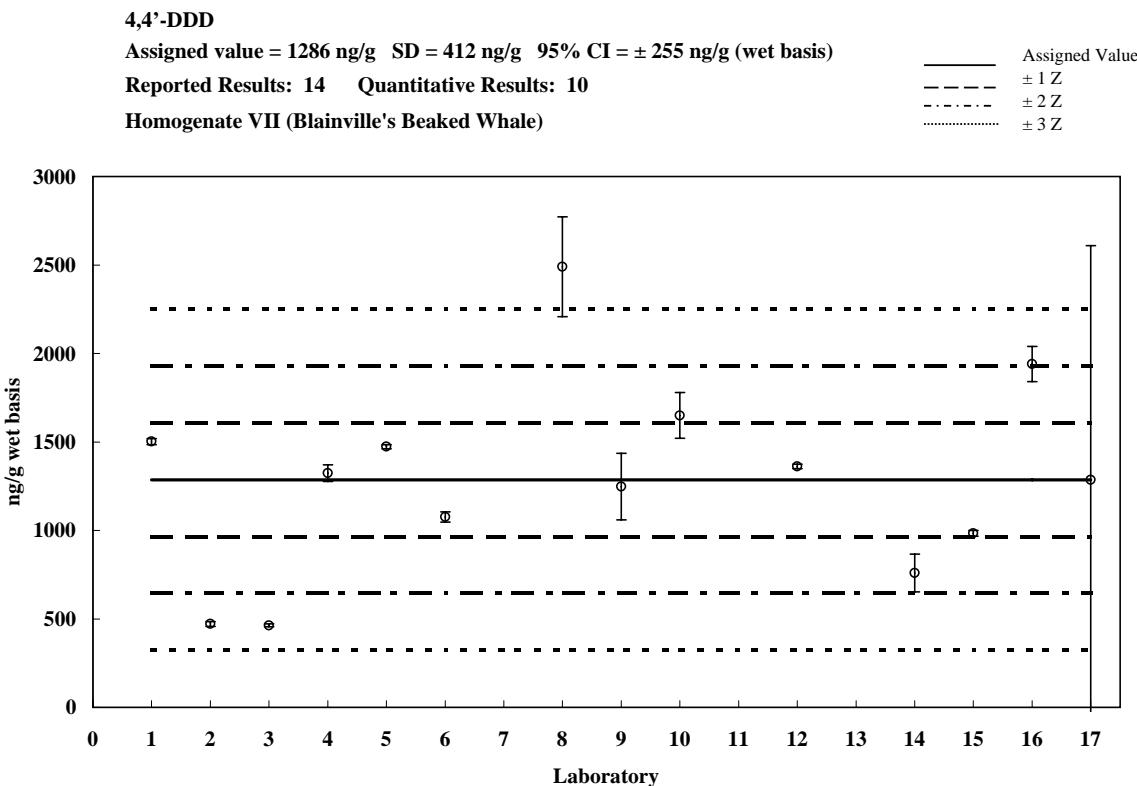

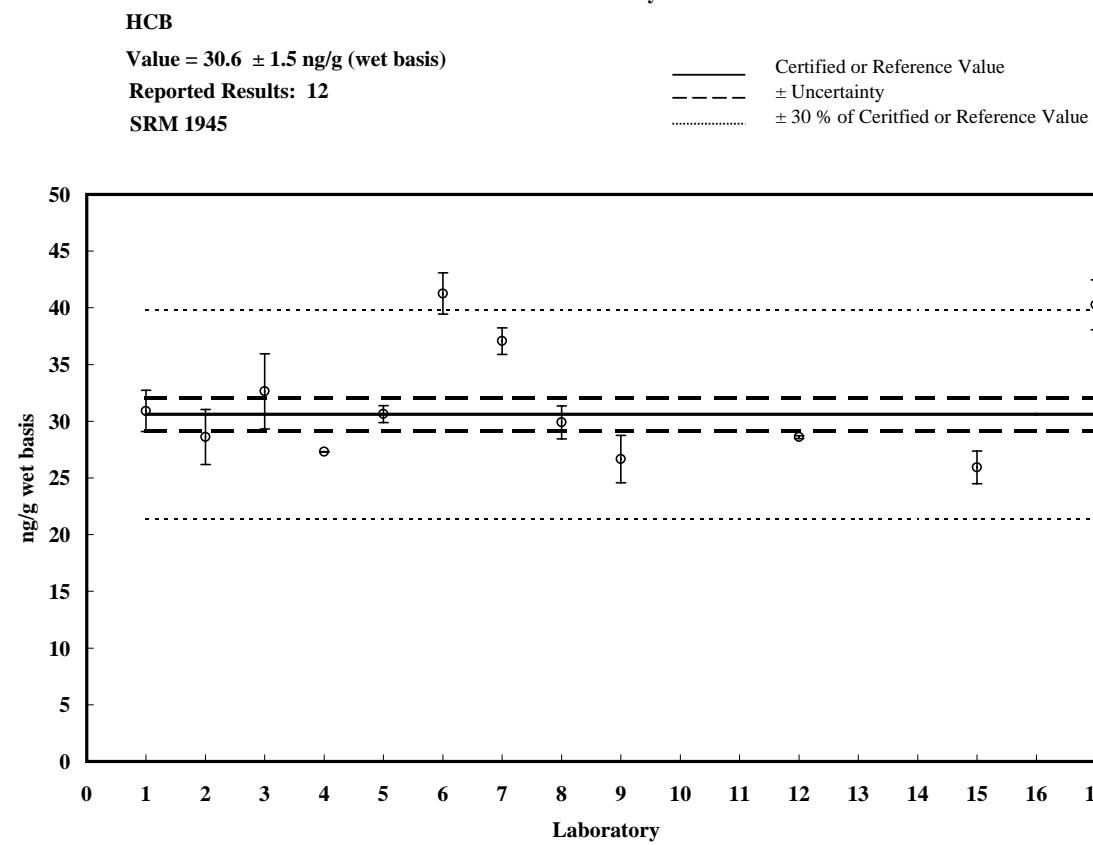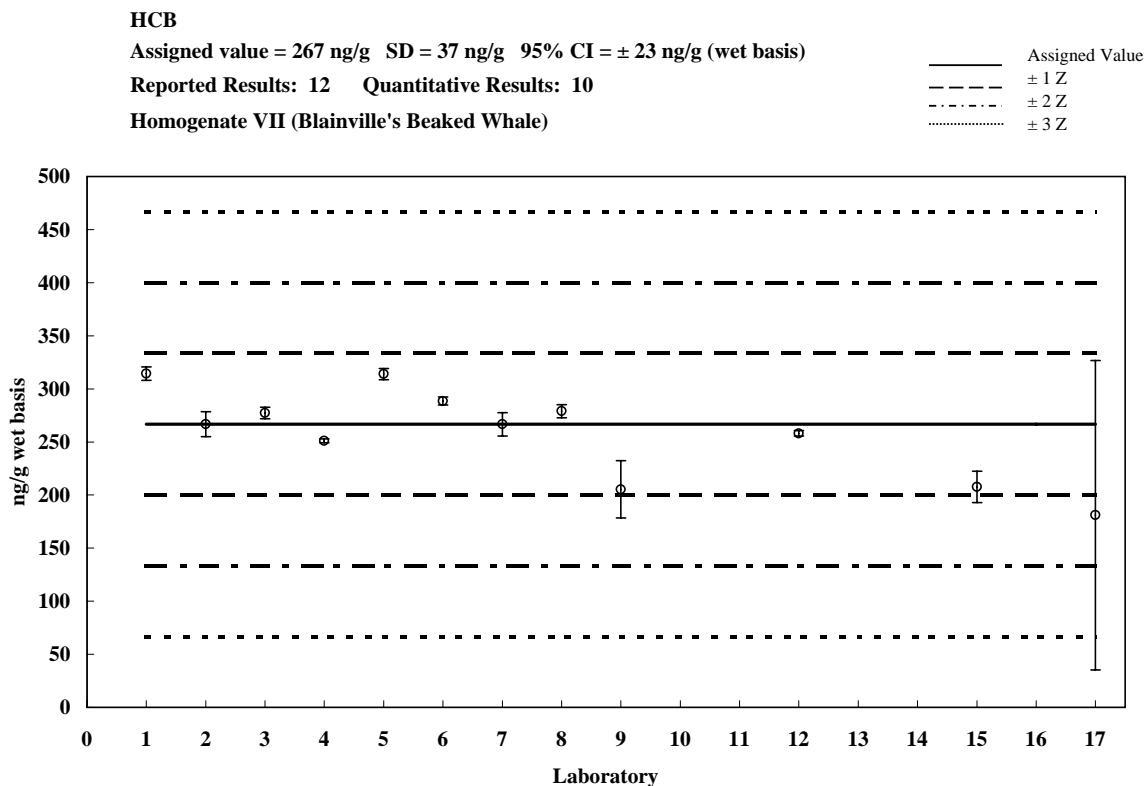


alpha-HCH

Assigned value = 4.12 ng/g SD = 1 ng/g 95% CI = \pm 1 ng/g (wet basis)

Reported Results: 4 Quantitative Results: 4

Homogenate VII (Blainville's Beaked Whale)

Assigned Value
 \pm 1 Z
 \pm 2 Z
 \pm 3 Z

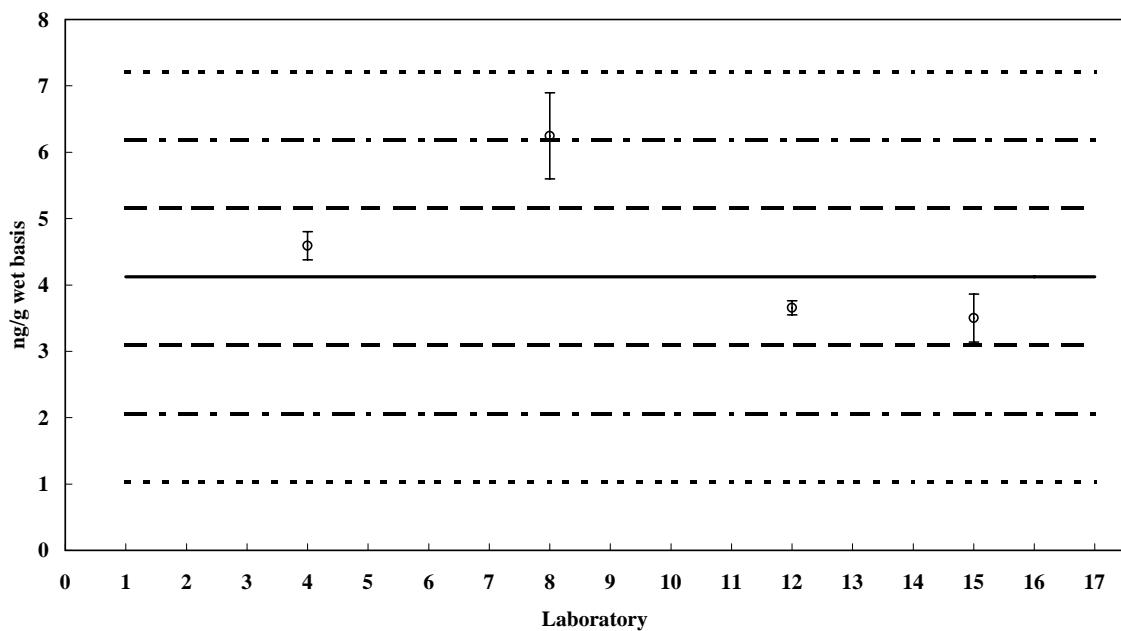


alpha-HCH



Value = 16.9 \pm 1.4 ng/g (wet basis)



Reported Results: 7



SRM 1945



Certified or Reference Value
 \pm Uncertainty
 \pm 30 % of Certified or Reference Value


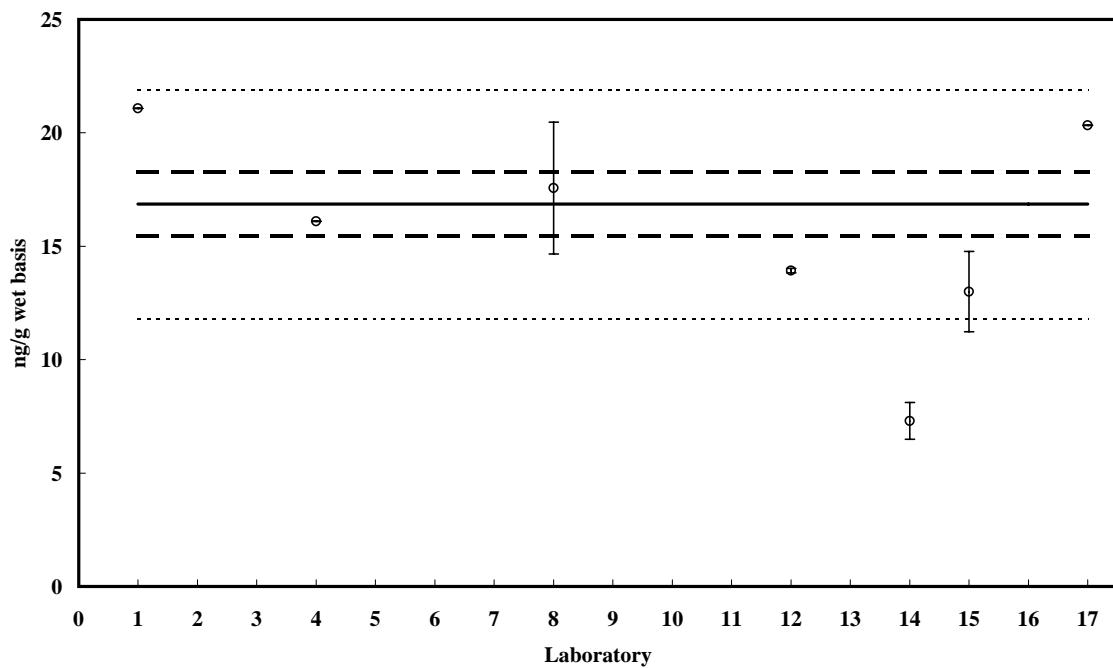


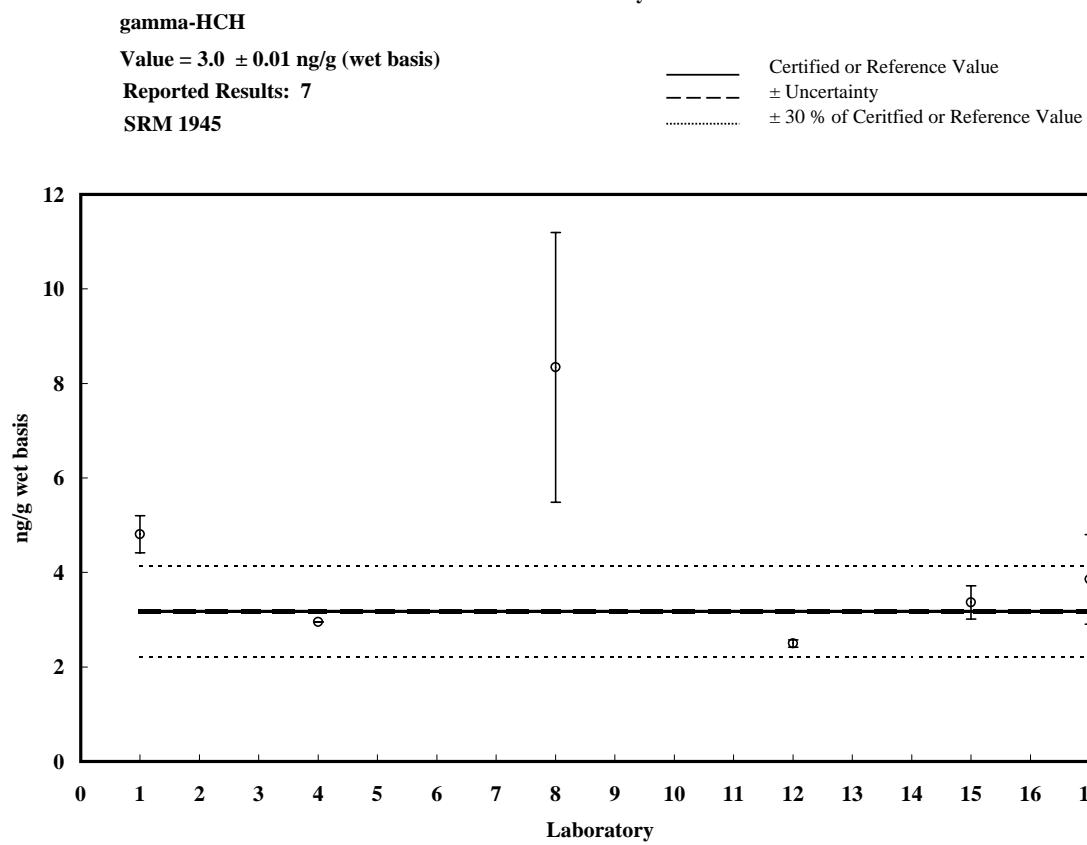
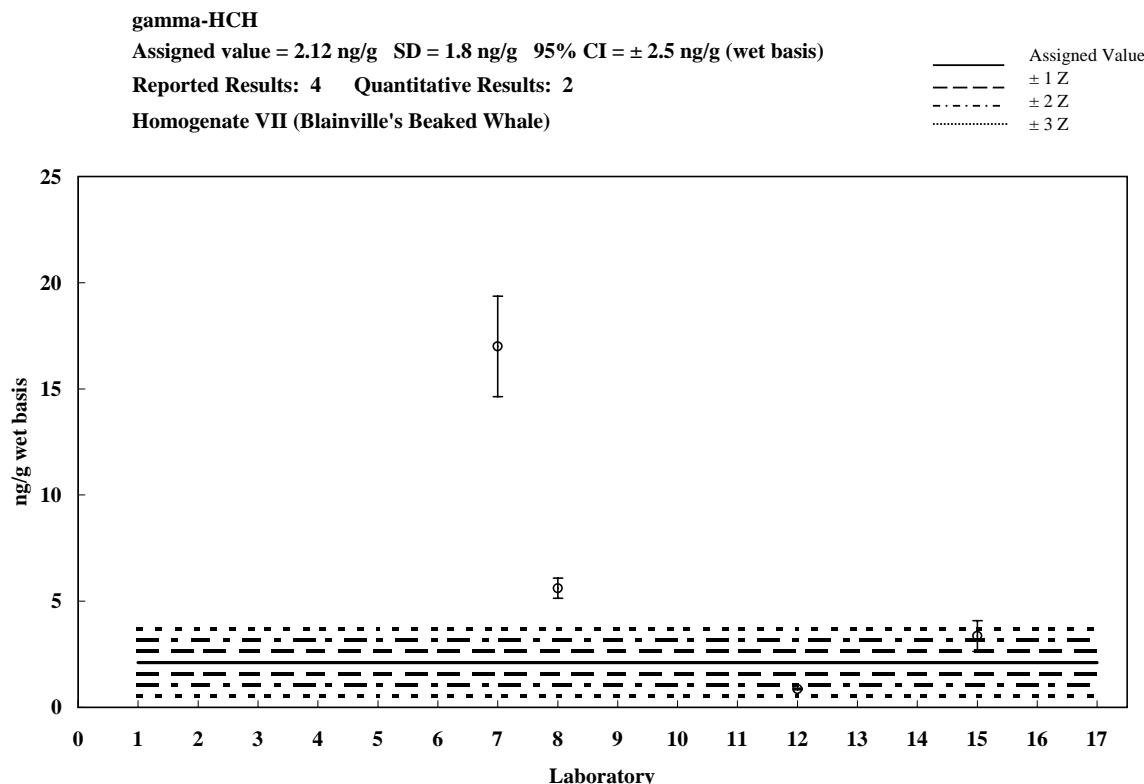


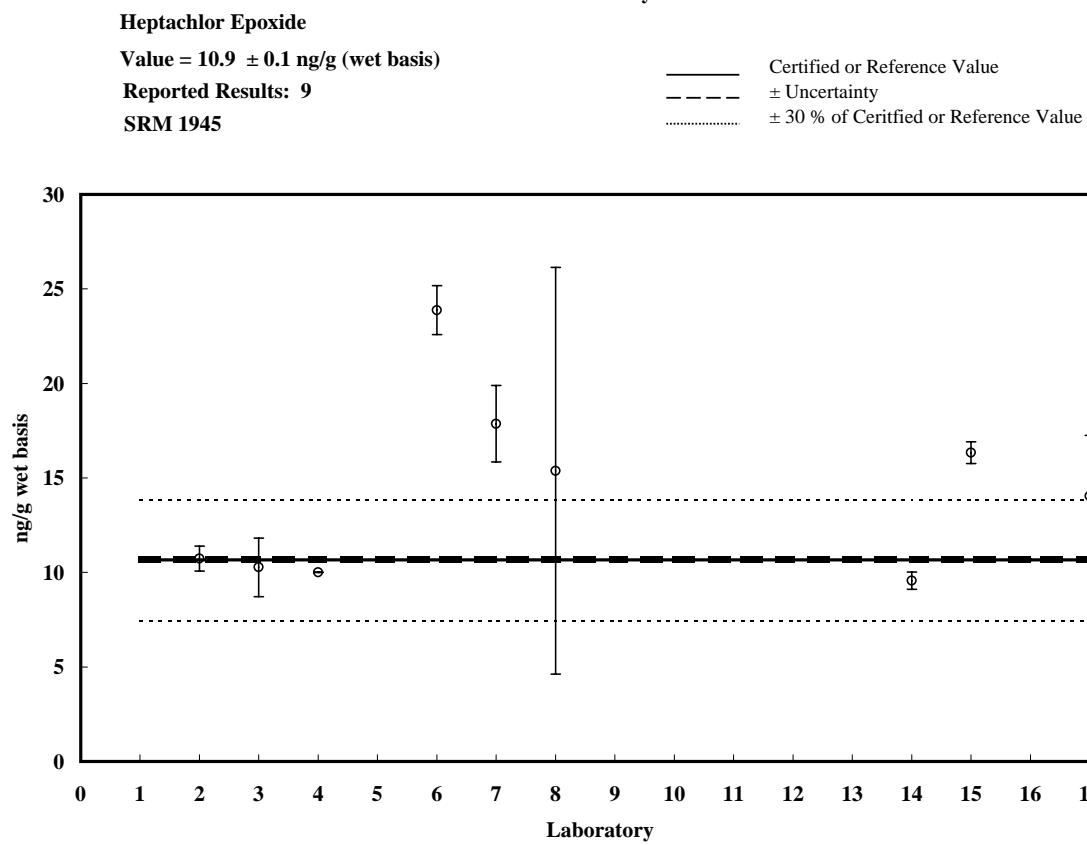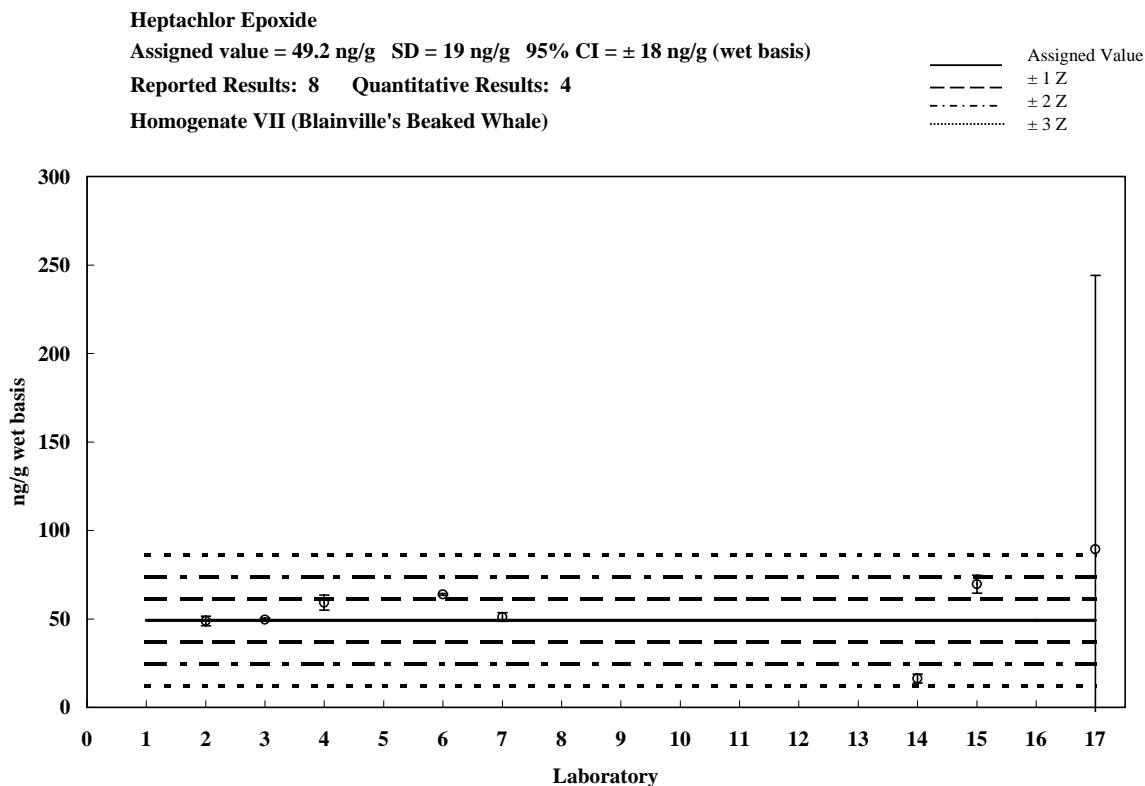


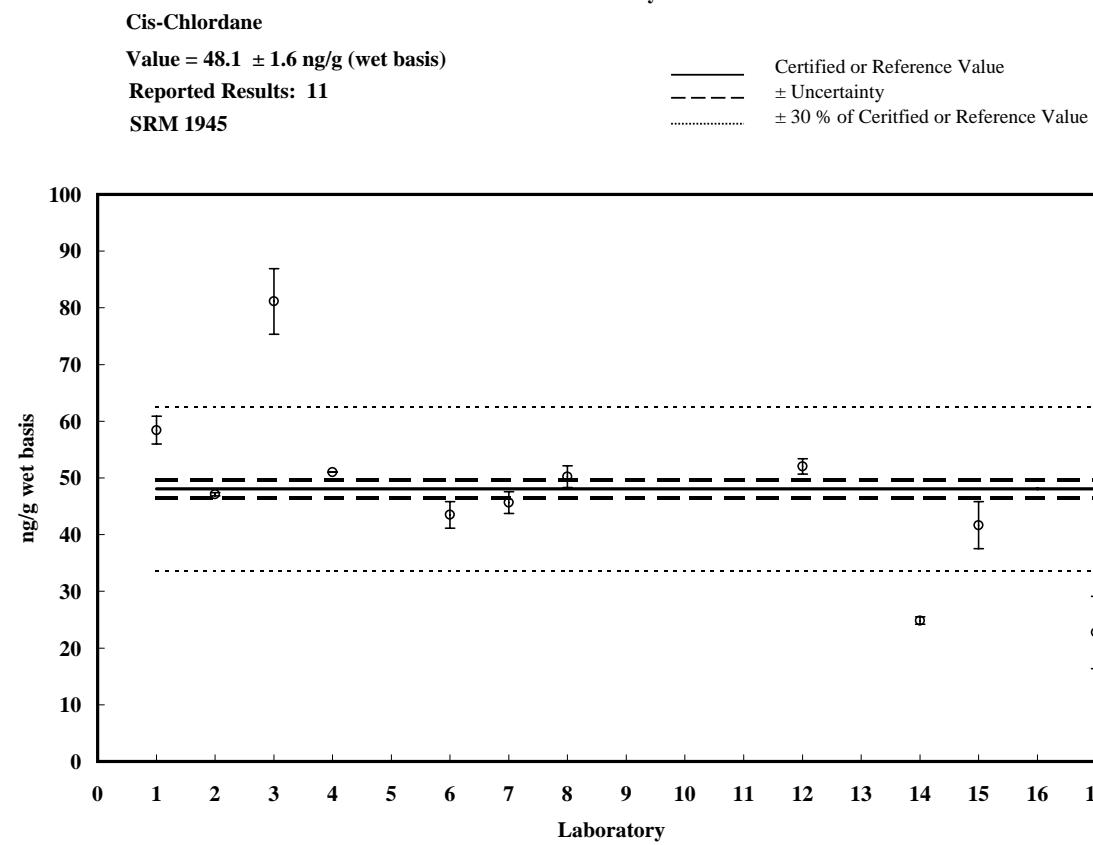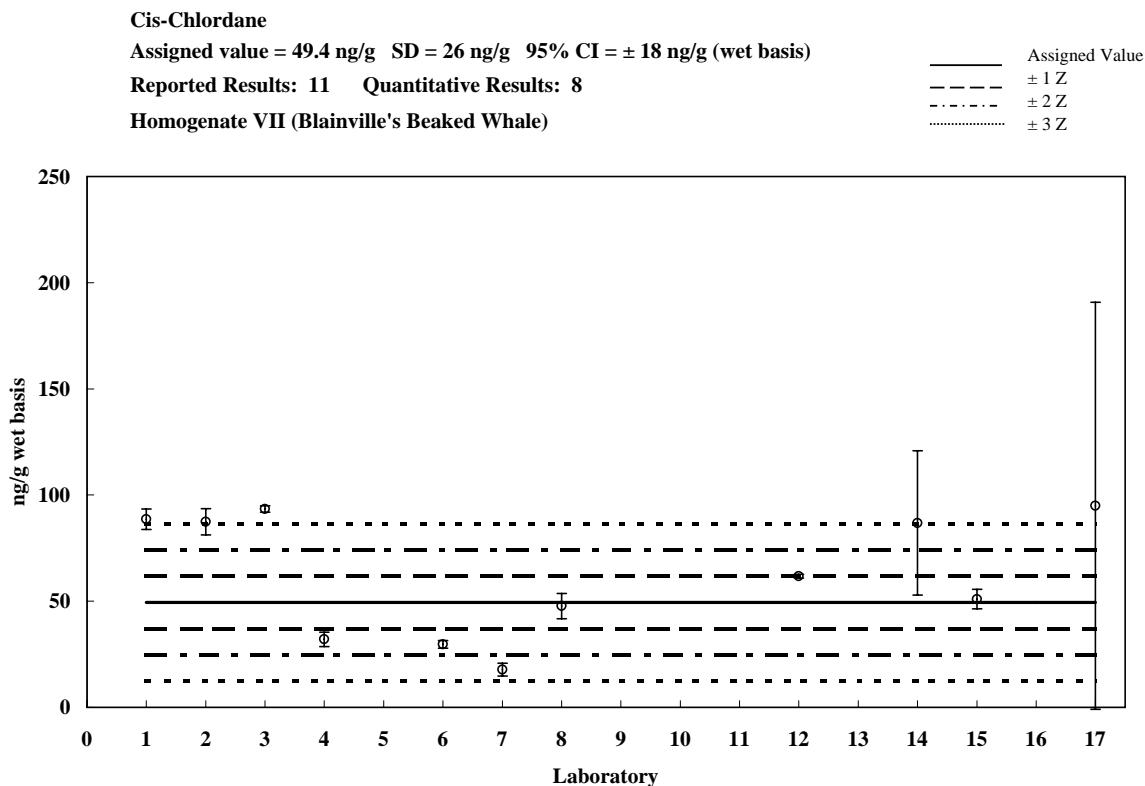


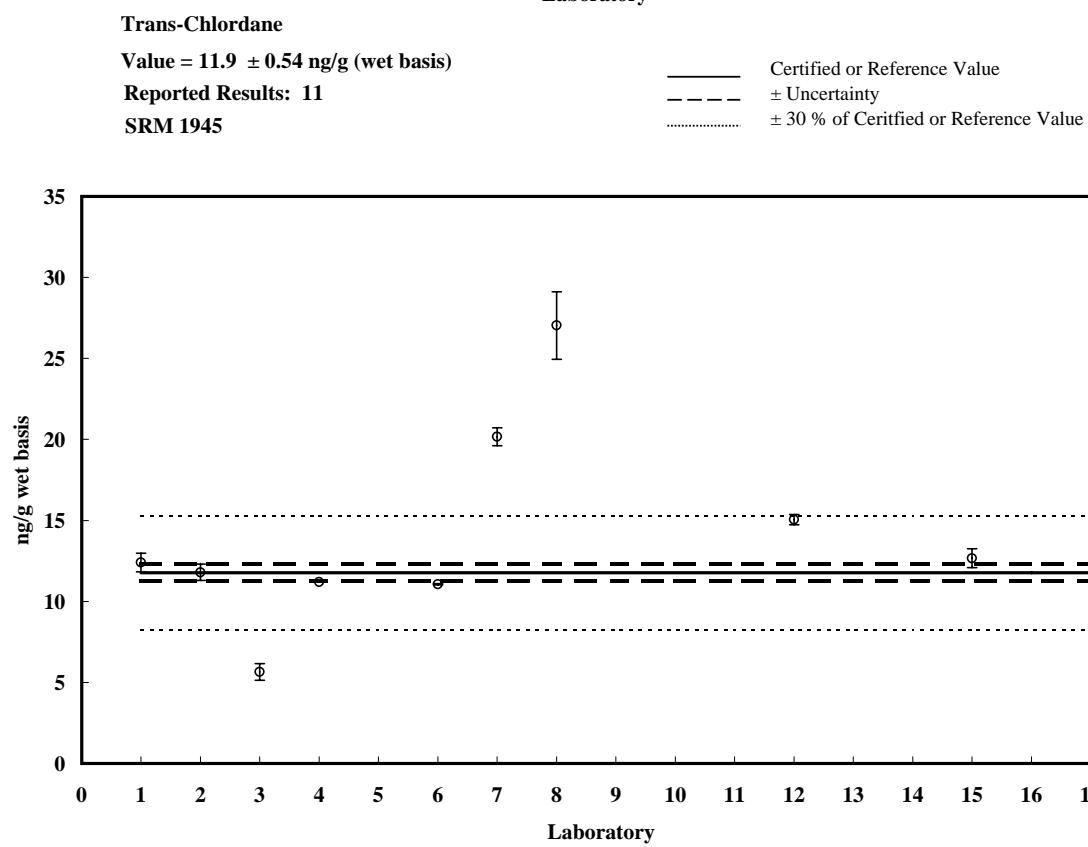
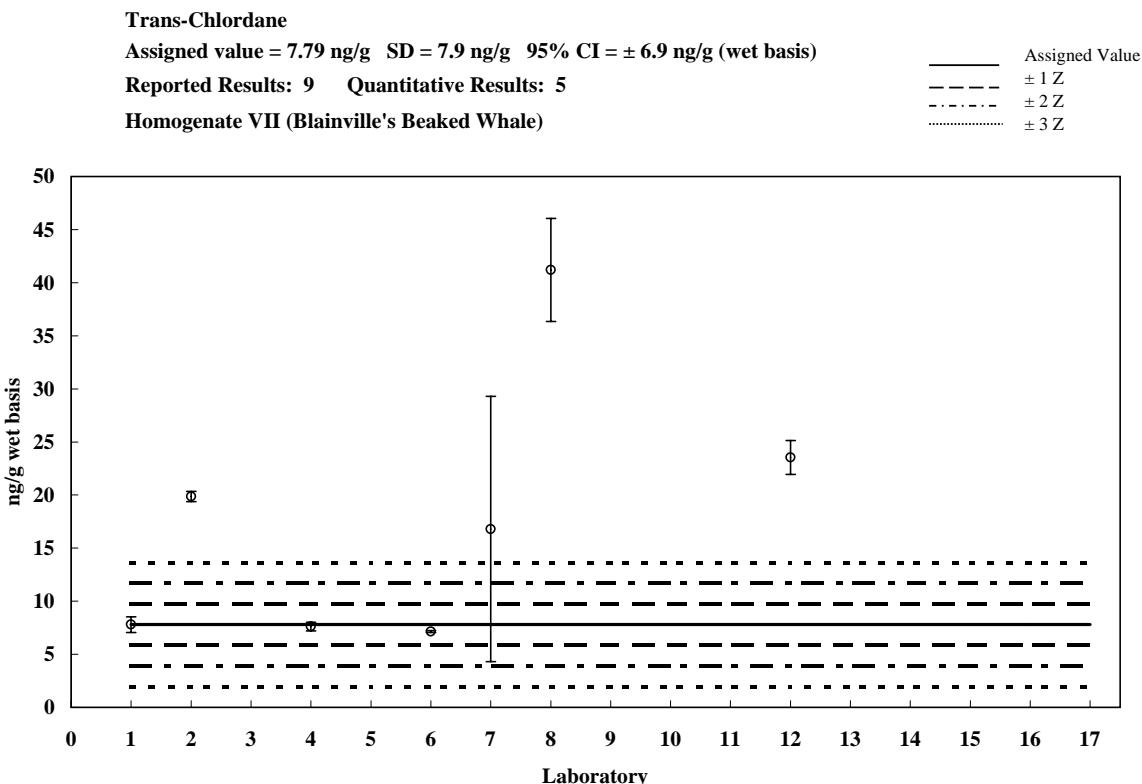


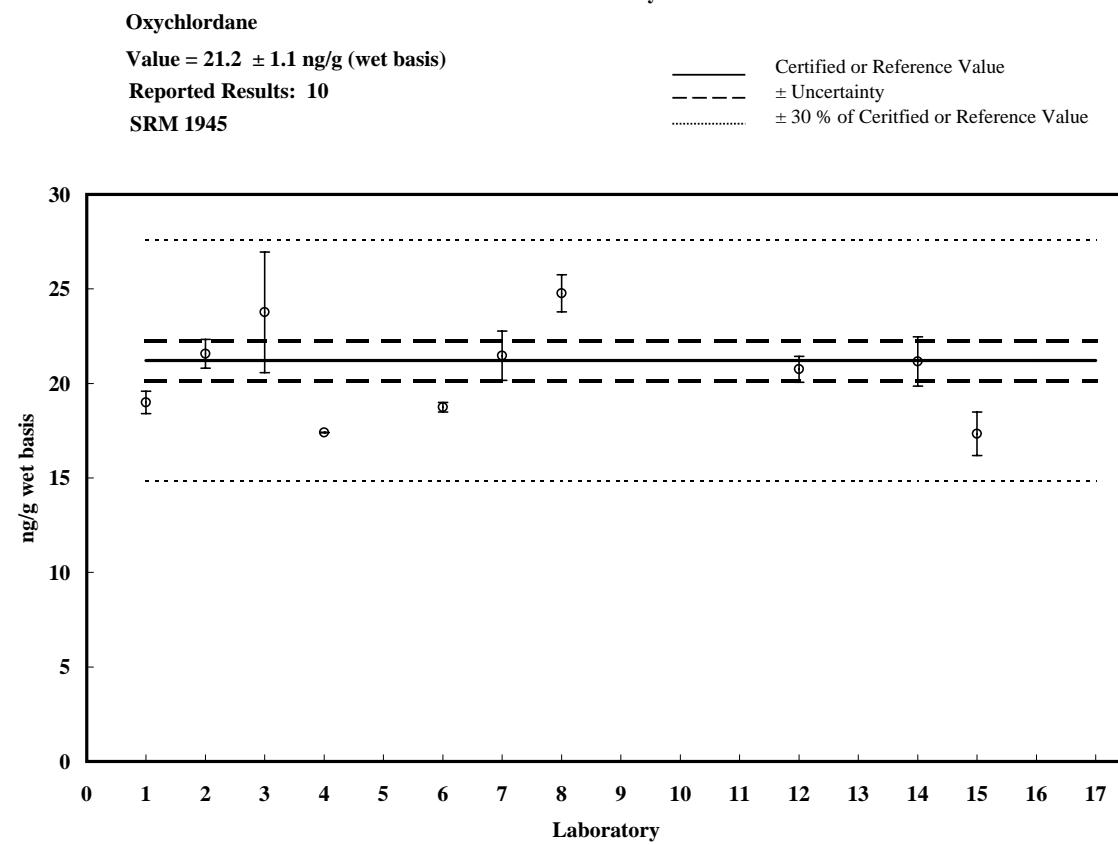
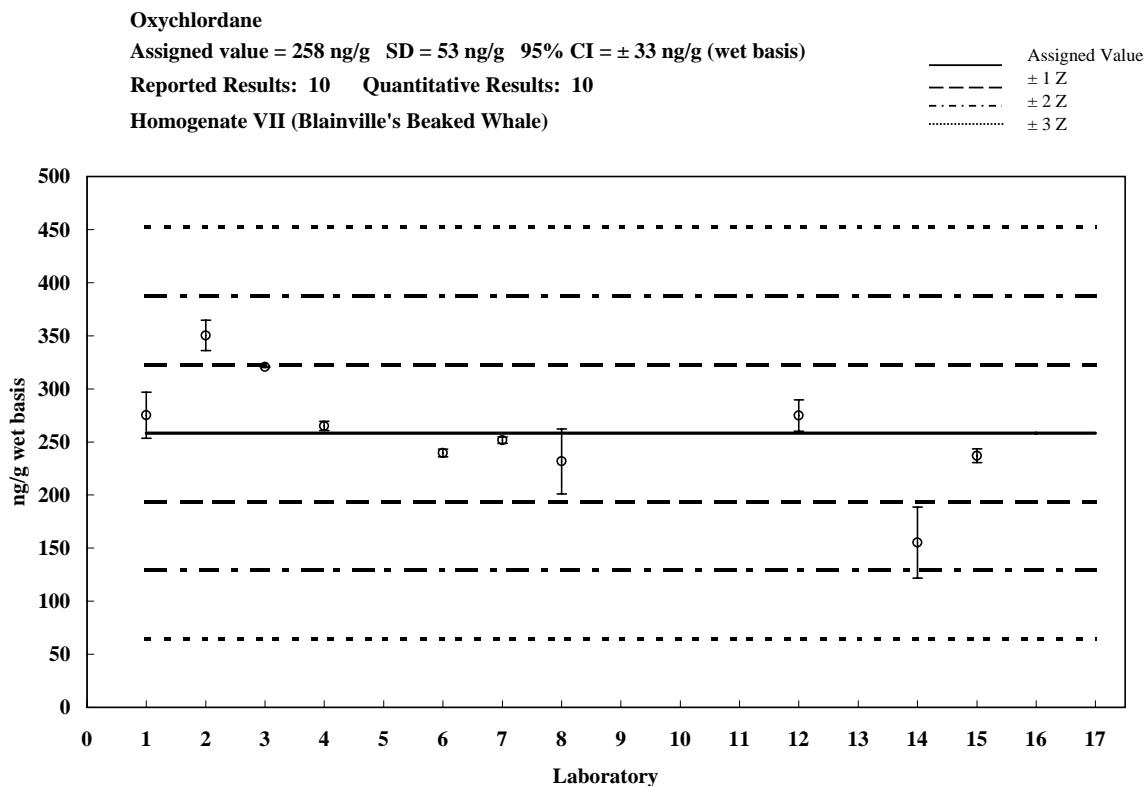


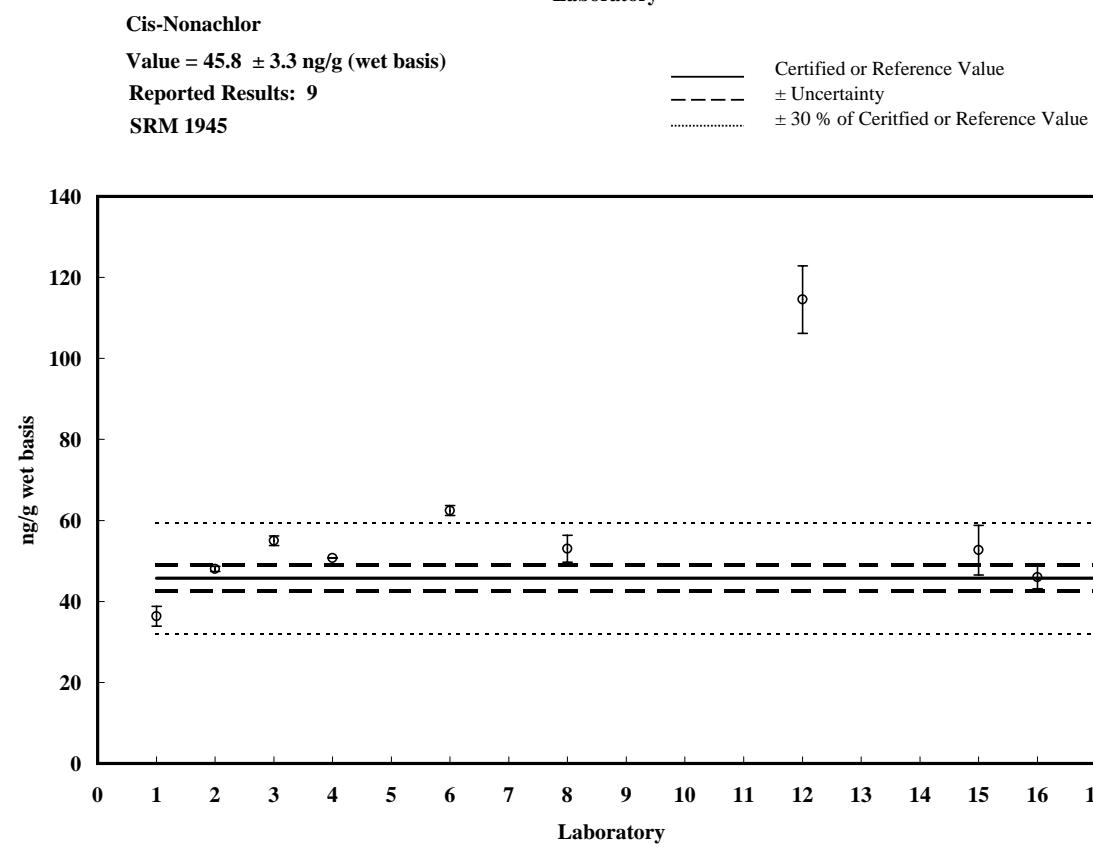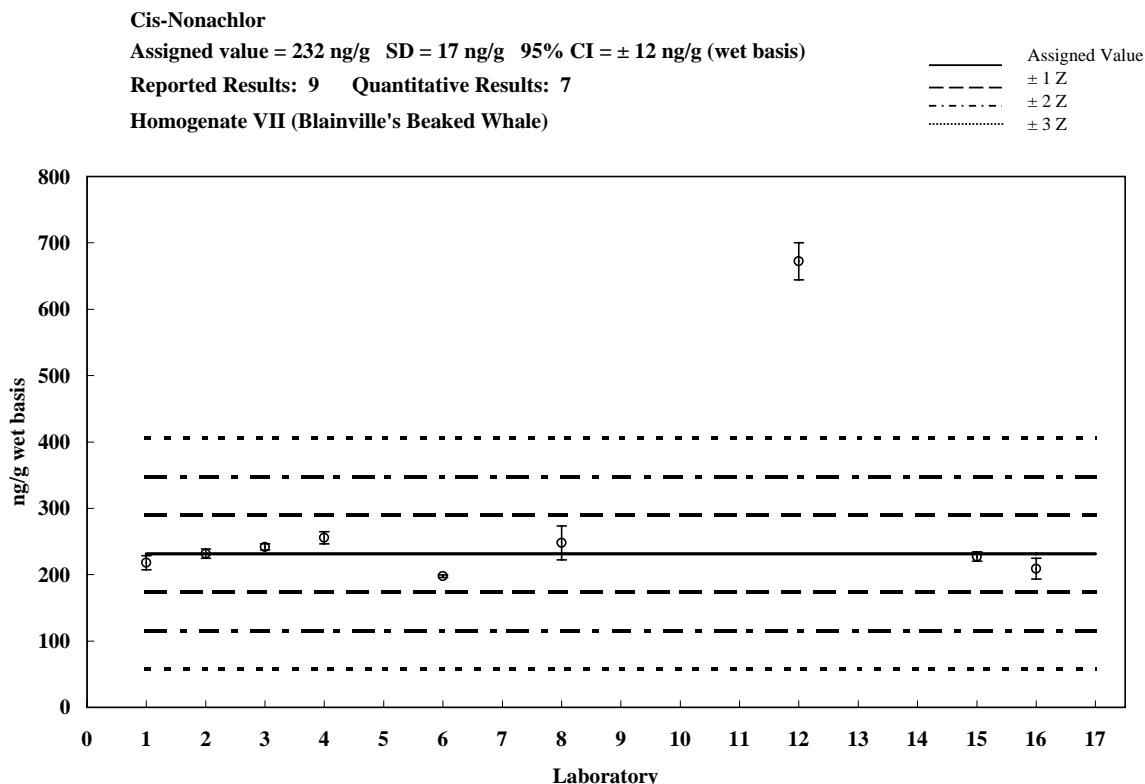

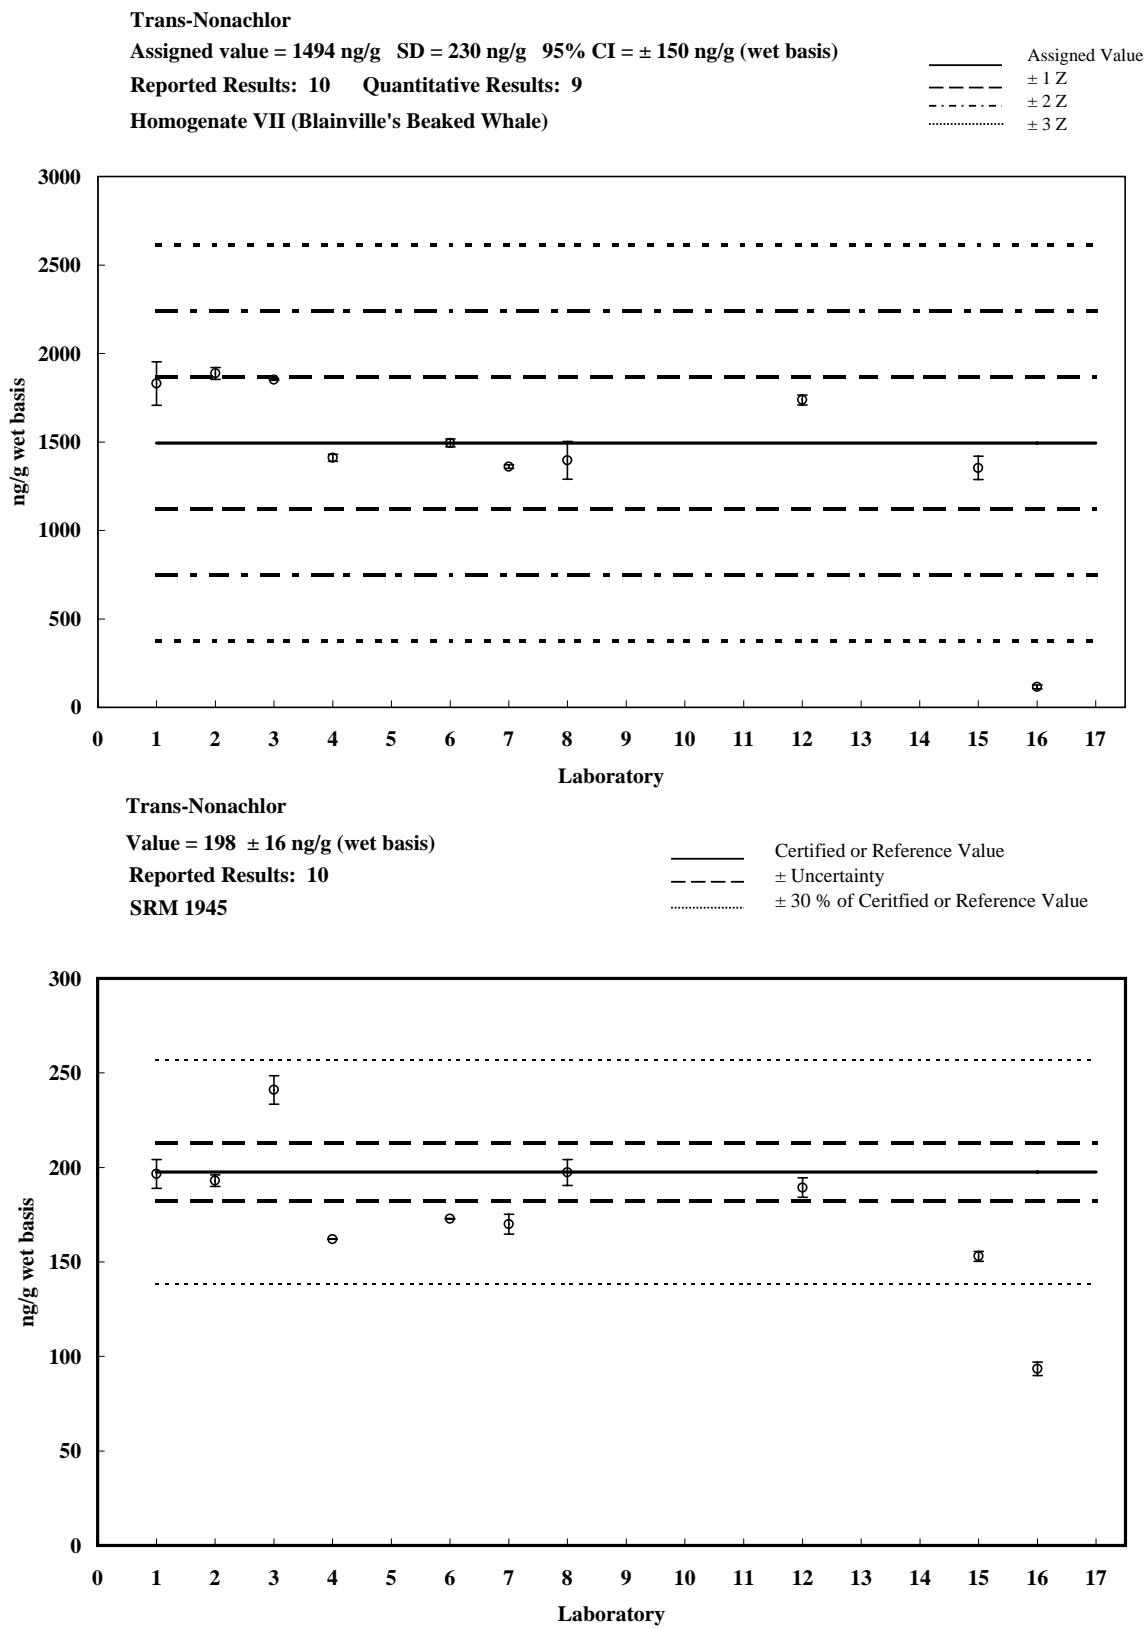

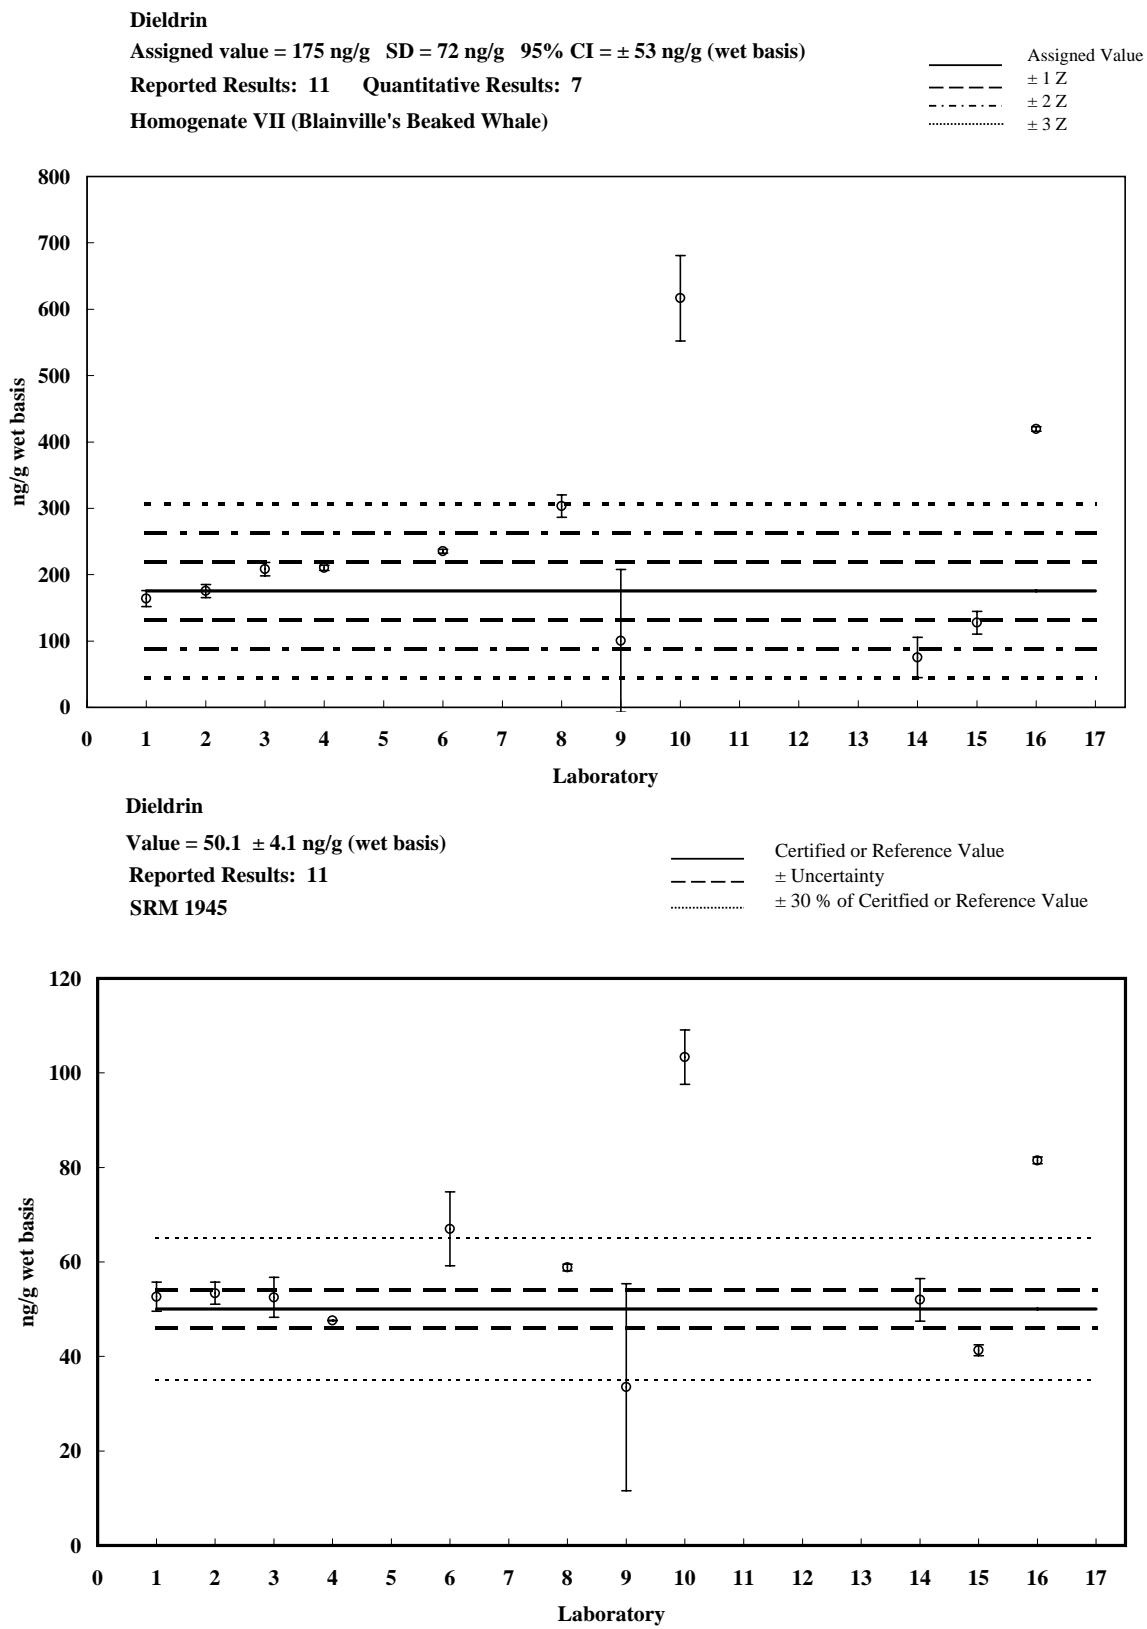

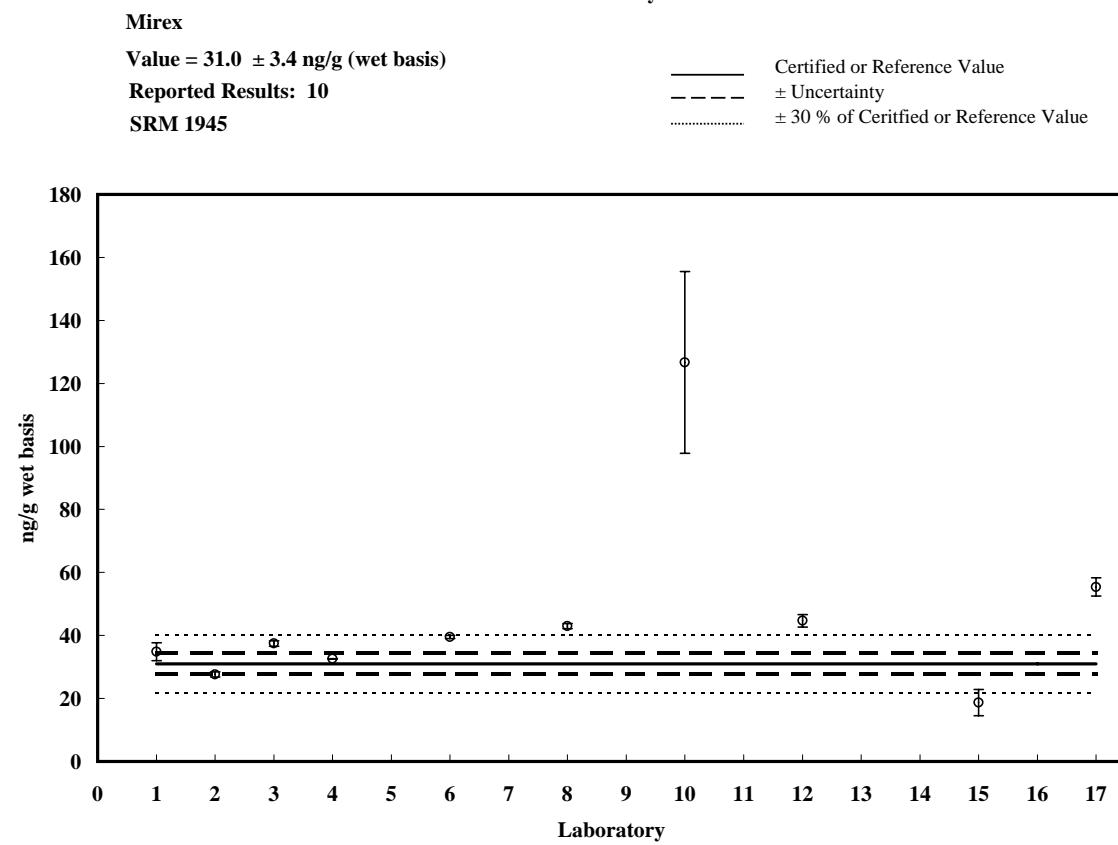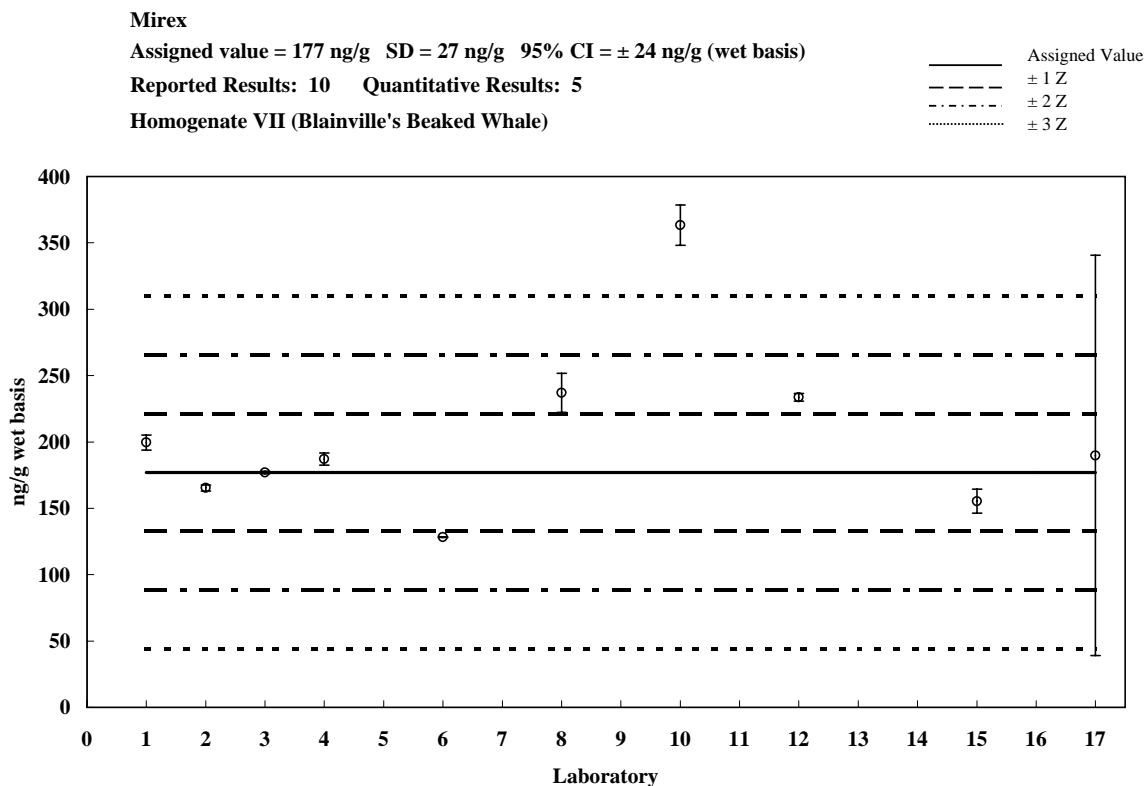

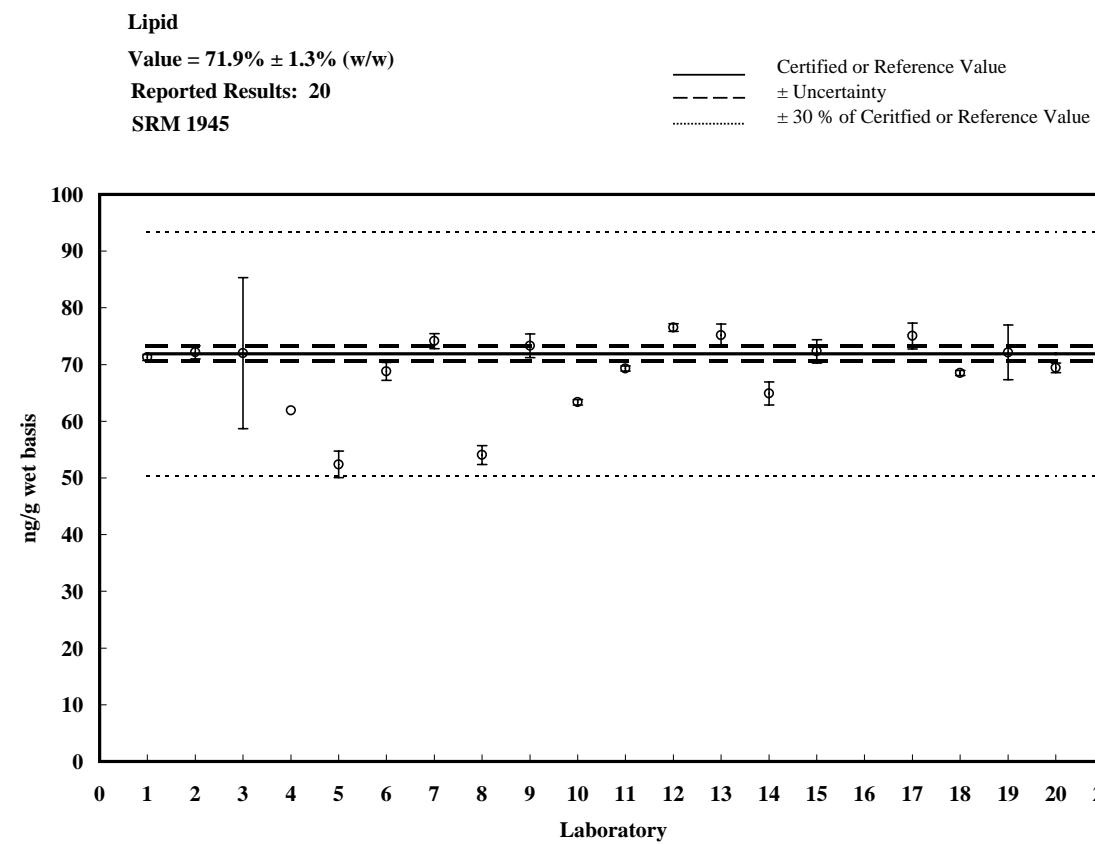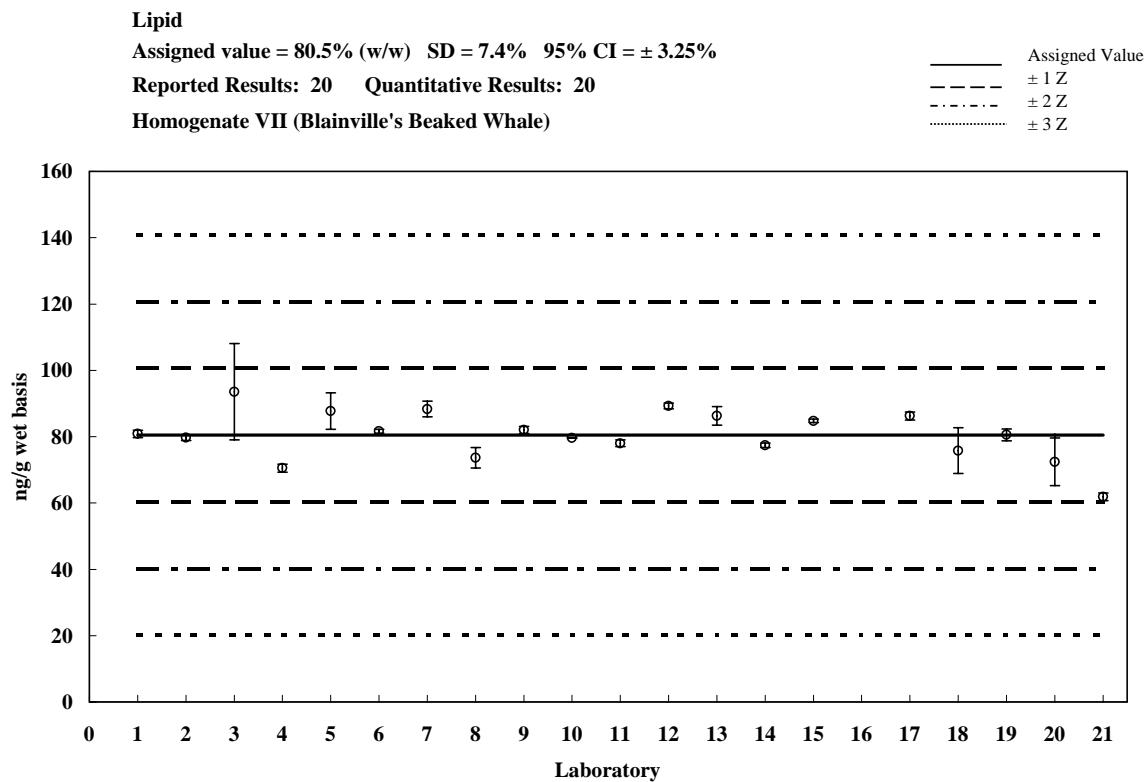

Appendix D


Graphical results of PBDE congener data reported by all laboratories. The Z-scores for Homogenate VII represent 25 % of the assigned value so that z = +1 is the assigned value plus 25 %, z = -1 is the assigned value minus 25 % and so forth. Error bars are \pm 1 standard deviation.

PBDE 47Assigned value = 132 ng/g SD = 132 ng/g 95% CI = \pm 9 ng/g (wet basis)

Reported Results: 8 Quantitative Results: 8

Control Material VII (Blainville's beaked whale)


Assigned Value
 \pm 1 Z
 \pm 2 Z
 \pm 3 Z

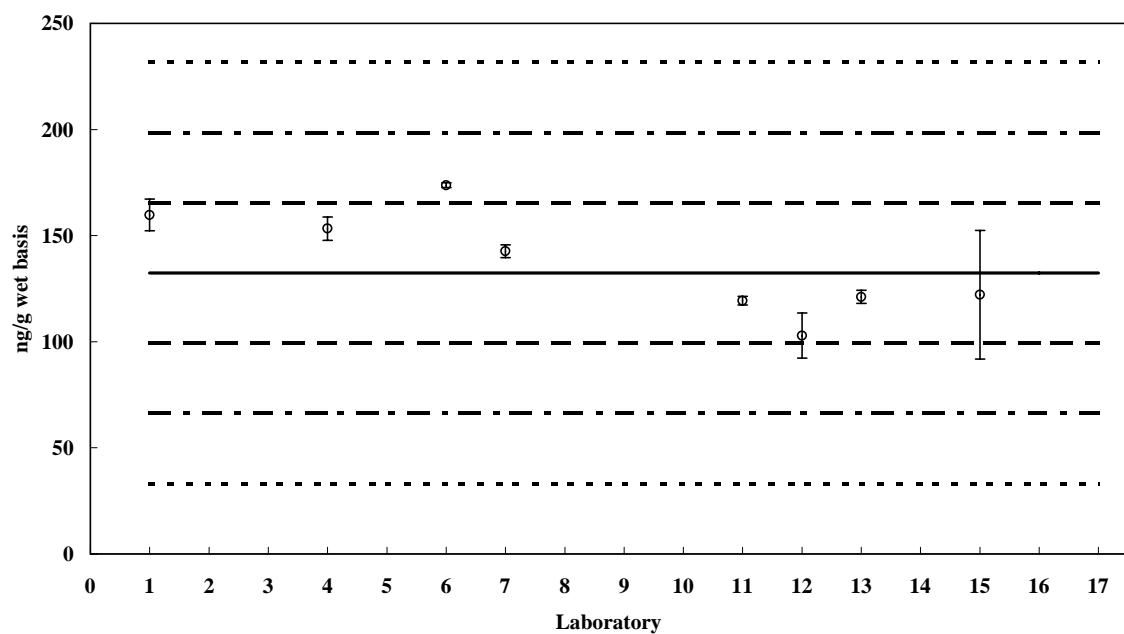**PBDE 47**Value = 39.6 \pm 0.2 ng/g (wet basis)

Reported Results: 8

SRM 1945

Certified or Reference Value
 \pm Uncertainty
 \pm 30 % of Certified or Reference Value

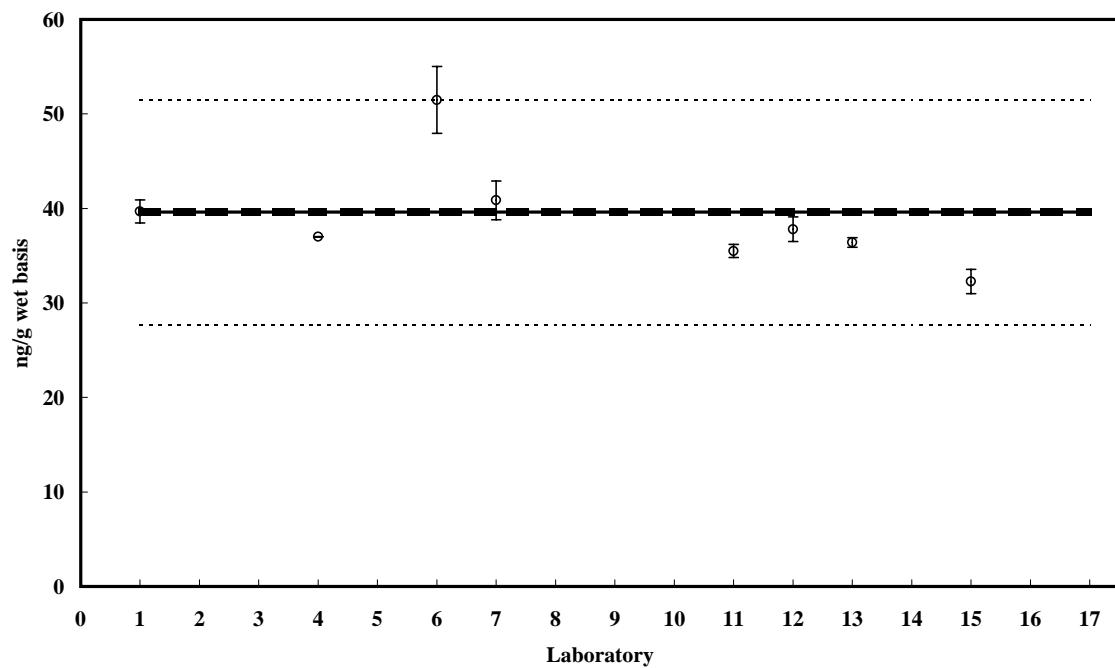


PBDE 99Assigned value = 22.2 ng/g SD = 3.2 ng/g 95% CI = \pm 2.8 ng/g (wet basis)

Reported Results: 7 Quantitative Results: 5

Control Material VII (Blainville's beaked whale)


____ Assigned Value
 - - - \pm 1 Z
 - - - \pm 2 Z
 - - - - \pm 3 Z

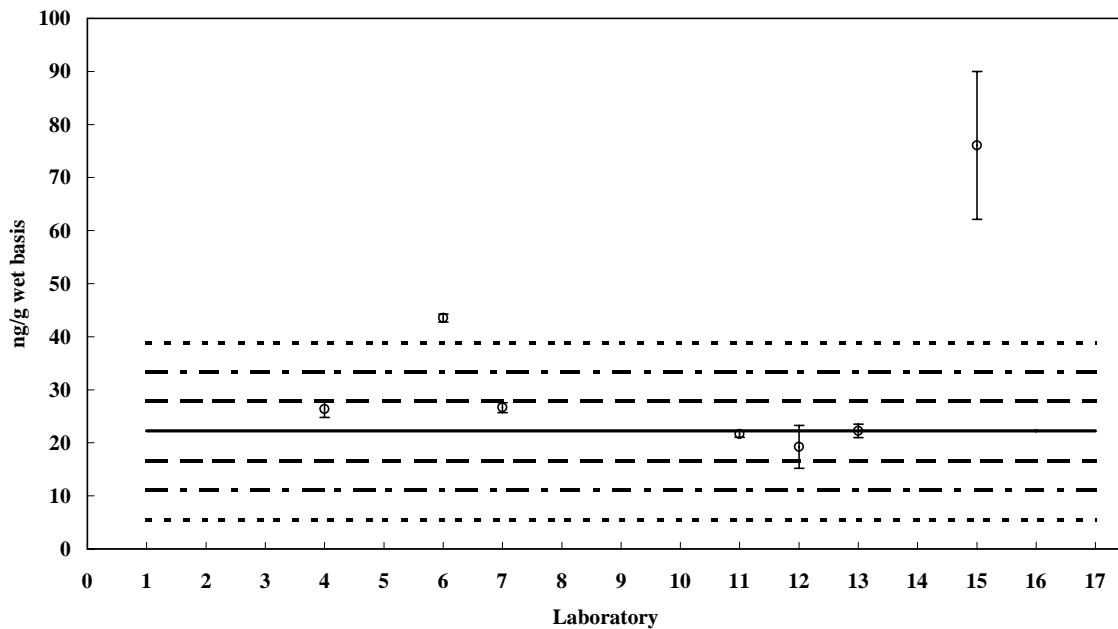**PBDE 99**Value = 18.9 \pm 2.3 ng/g (wet basis)

Reported Results: 7

SRM 1945

____ Certified or Reference Value
 - - - \pm Uncertainty
 - - - - \pm 30 % of Certifid or Reference Value

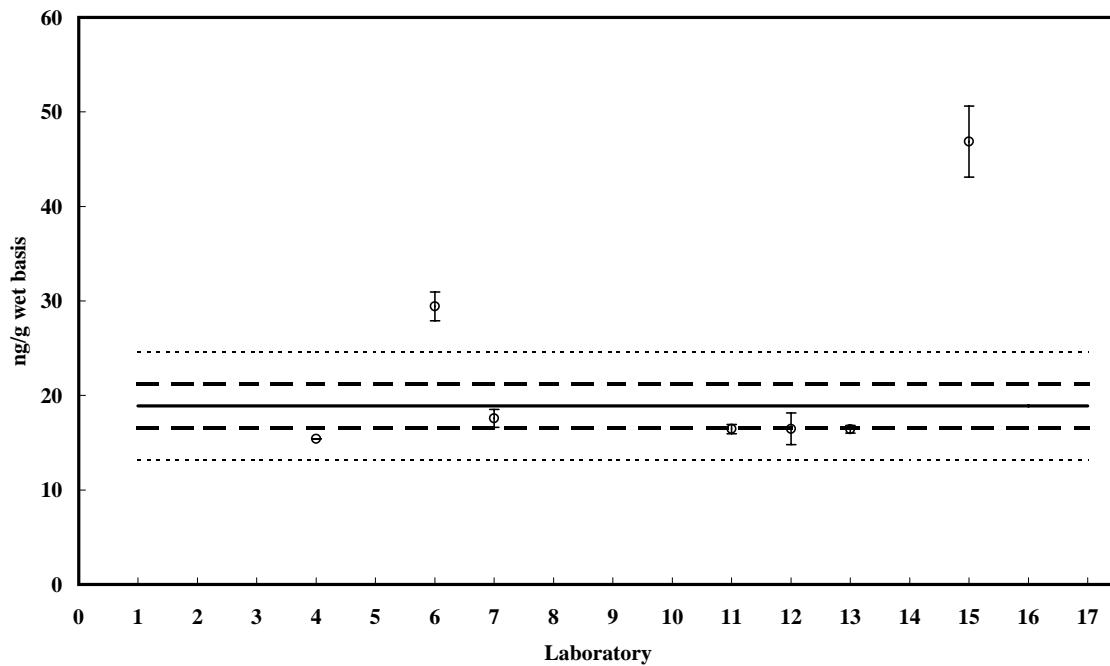


PBDE 100Assigned value = 40 ng/g SD = 8.2 ng/g 95% CI = \pm 6.1 ng/g (wet basis)

Reported Results: 8 Quantitative Results: 7

Control Material VII (Blainville's beaked whale)


____ Assigned Value
 - - - \pm 1 Z
 - - - \pm 2 Z
 \pm 3 Z

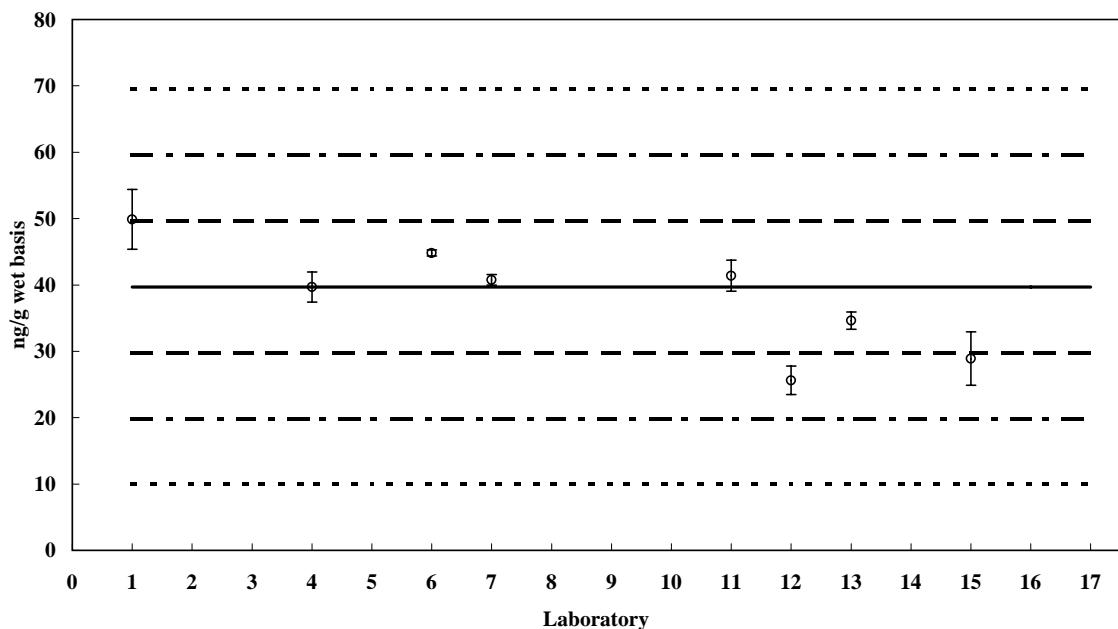**PBDE 100**Value = 10.3 \pm 1.1 ng/g (wet basis)

Reported Results: 8

SRM 1945

____ Certified or Reference Value
 - - - \pm Uncertainty
 \pm 30 % of Certified or Reference Value

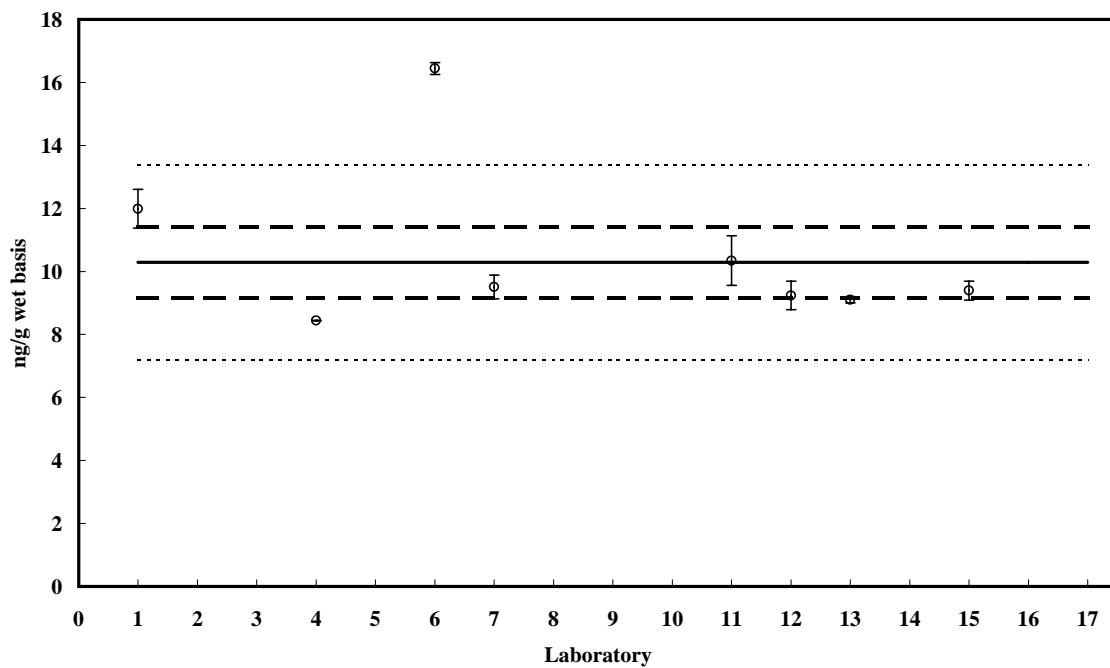


PBDE 153Assigned value = 14.2 ng/g SD = 2.0 ng/g 95% CI = \pm 1.6 ng/g (wet basis)

Reported Results: 8 Quantitative Results: 6

Control Material VII (Blainville's beaked whale)


Assigned Value
 \pm 1 Z
 \pm 2 Z
 \pm 3 Z

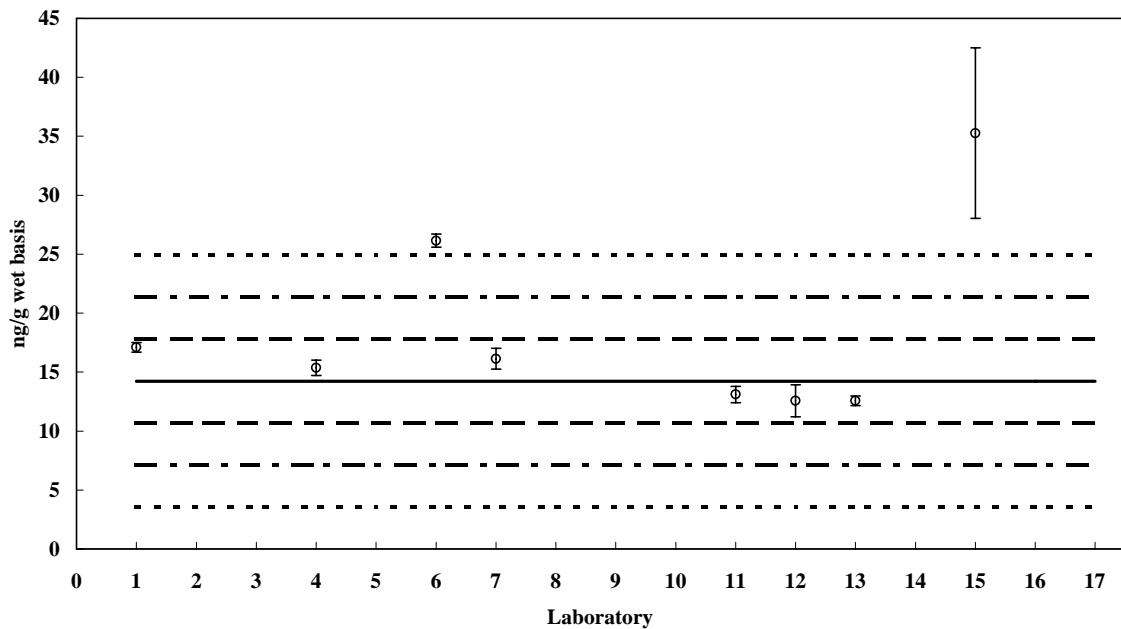**PBDE 153**Value = 8.3 \pm 0.6 ng/g (wet basis)

Reported Results: 8

SRM 1945

Certified or Reference Value
 \pm Uncertainty
 \pm 30 % of Certified or Reference Value

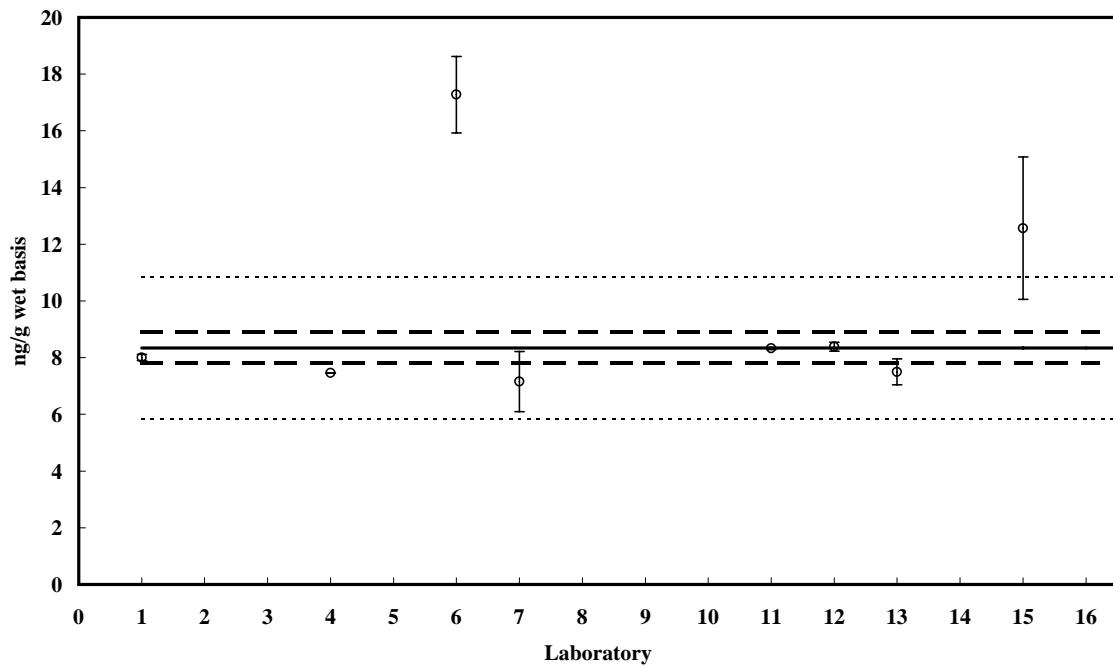


PBDE 154Assigned value = 36.7 ng/g SD = 9.4 ng/g 95% CI = \pm 7.5 ng/g (wet basis)


Reported Results: 8 Quantitative Results: 6

Control Material VII (Blainville's beaked whale)

Assigned Value
 \pm 1 Z
 \pm 2 Z
 \pm 3 Z

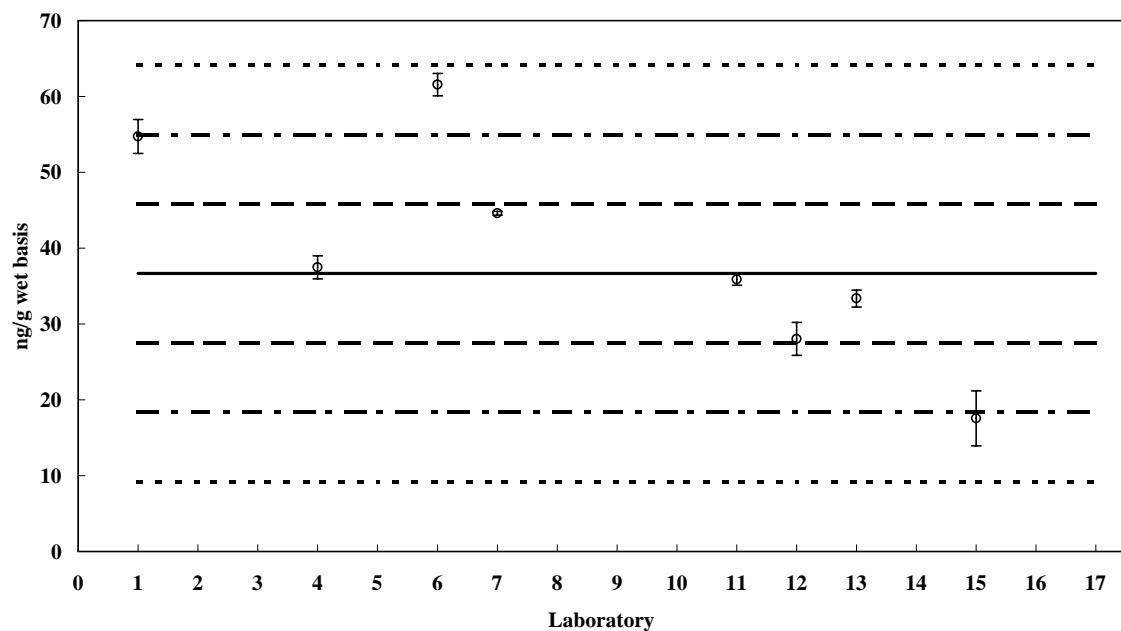**PBDE 154**Value = 13.3 \pm 1.7 ng/g (wet basis)**SRM 1945**

Certified or Reference Value
 \pm Uncertainty
 \pm 30 % of Certified or Reference Value

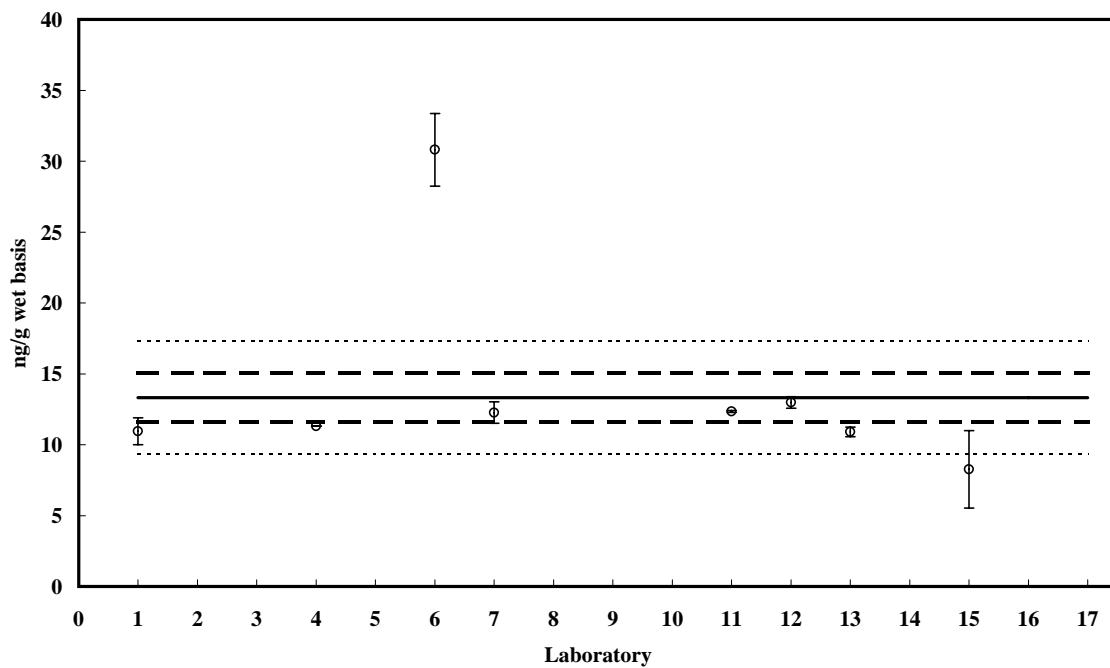

Appendix E

Tabular summary of methods used for analysis by each laboratory.

Summary of Methods Used

Laboratory	Approximate mass of sample extracted (g):		Procedure used to measure Lipid	Were "wet" or "dry" samples extracted?	
	SRM 1945	Homog. VII		SRM 1945	Homog. VII
1	1	1	Subsampled the dichloromethane extract, evaporated the solvent and weighed the remaining residue	wet	wet
2	1.5	1.5	gravimetric - using 100 µL aliquot of extract	wet	wet
3	1	1	removed aliquot and allowed to air dry	wet	wet
4	1	1	Gravimetric determination; ASE extraction using dichloromethane.	wet	wet
5	0.3	0.3	Accelerated solvent extraction (ASE) with dichloromethane and quantitation by thin-layer chromatography with flame ionization detection (TLC-FID) for total lipid and lipid classes.	wet	wet
6	1	1	Gravimetric	wet	wet
7	3.17 to 4.03	3.65 to 5.52	After extraction with dichloromethane, the extracts of Homognate VII were concentrated to 10ml. The extracts of SRM 1945 were relatively lipid rich and were concentrated to 25ml. Then, 20% by volume of these extracts was added to a previously weighed and dried aluminum pan. The contents were allowed to evaporate, and the pan was reweighed. See note 1 at the end of this report for additional comments	wet	wet
8	0.6	0.7	Weighing aloquot of methylene chloride extract	wet	wet
9	1	1	Gravimetric	wet	wet
10	3	5	Total extractable lipids (gravimetric from Soxhlet extract)	wet	wet
11	2.25-3.02	2.54-3.62	Gravimetric determination from portion of the Soxhlet extraction.	wet	wet
12	1	1	evaporation of the lipid extract is done under a stream of Nitrogen	wet	wet
13	0.15	0.12	Samples were mixed with sodium sulphate and Soxhlet extracted. Lipids were determined on an aliquot of the extract (~1/6) after solvent evaporation at 105° for 1h	wet	wet
14	1	1		wet	wet
15	1	1		wet	wet
16	2	2		wet	wet
17	0.591	0.593	Accelerated solvent extraction with methylene chloride. Heat for 6 minutes in 125 Celsius oven at 2000 psi UHP nitrogen. Static hold of 4 minutes followed by 60% flush for 120 seconds.	wet	wet
18	0.278	0.348	Extract is brought to a fixed volume (1ml) volumetrically by adding chloroform, then 50% of the extract is panned out and dried until moisture loss is negligible. % Lipid is then determined gravimetrically	wet	wet
19	1	1	Lipid composition: TLC indicated that SRM-1945 was primarily triacylglycerol and QC05WB7 primarily wax esters.	wet	wet
20	1	1	NOAA Sampling an Analytical Method of the National Status and Trends Program NOAA Technical Memorandum NOS ORCA 130	wet	wet
21	1	1	Gravimetric determination; ASE extraction using dichloromethane.	wet	wet

Summary of Methods Used

Laboratory	Extraction Method	Extraction Solvent	Extraction Time	Extraction Other	Sample Extract Cleanup Method
1	Pressurized Fluid Extraction (Dionex, ASE)	Dichloromethane	15 min	Sample dried with 45 g sodium sulfate, then packed into a 33 mL PFE cell. PFE Conditions: cell temp 100 °C. equilibration 5 min, static time 5 min, cell pressure 2000 psi and there were three cycles. Samples were first run through a Gel Permeation chrom.	Samples were first run through a size exclusion chromatograph (SEC) column (Phenomenex) using DCM as the mobile phase. Eluent containing organochlorines was further refined by passing though a ca. 2 g alumina solid phase extraction cartridge eluting with 12 mL 25% DCM:75% hexane (volume fraction).
2	Pressurized Fluid Extraction (Dionex, ASE)	Dichloromethane	15 min	100 °C; 2000 psi, 3 cycles; 9(in hexane.	Size exclusion chromatography followed by solid phase extraction clean-up using silica SPE with 15 mL of 10 % DCM
3	Soxhlet	Dichloromethane	Overnight		Size exclusion chromatography followed by silica solid phase extraction cartridges with 15 mL of 25 % methylene chloride in hexane solid phase extraction procedure was repeated (as above) followed by size-exclusion chromatography (as above) a second time and a final solid phase extraction (as above).
4	Pressurized Fluid Extraction (Dionex, ASE)	Dichloromethane	16 min	ASE Conditions: Pressure = 2000 psi, temp = 100 °C	Gravity flow column with silica and neutral alumina, followed by HPLC-SEC to elute AH/CH fraction.
5	Pressurized Fluid Extraction (Dionex, ASE)	Dichloromethane	17 min	ASE Conditions: Pressure = 2000 psi, temp = 100 °C	Acidic/basic/neutral silica gel column (see Krahn et al. 1994 Chemosphere).
6	Pressurized Fluid Extraction (Dionex, ASE)	Dichloromethane	20 min		SX-2 Biobeads, Size exclusion Chromatography/dichloromethan. Florisil adsorptive chromatography/20% Ethyl/Petroleum Ether.

Summary of Methods Used

Laboratory	Extraction Method	Extraction Solvent	Extraction Time	Extraction Other	Sample Extract Cleanup Method
7	Soxhlet	Dichloromethane	18 hours		Each extract was eluted through a glass chromatography column packed with florisil, alumina, and silica and was concentrated to 10mL. A single, 2 mL portion of this eluate was diluted to 5 mL with methylene chloride. The unused portion of each sample was stored away as a reserve. Each 5 mL portion was manually injected into a single Phenogel, size exclusion HPLC column (60 cm x 2.1 cm). Each HPLC-cleaned fraction was concentrated, the solvent was exchanged to hexane, and the sample volume was adjusted to 5mL for initial GC screening. After screening, each sample was concentrated to 1mL for final data collection.
8	Tissuemizer with Na ₂ SO ₄	Dichloromethane	3 x 3 min		Silica/alumina column; HPLC phenogel
9	Soxhlet	Hexane:Acetone 1:1	4-6 hours		Alumina cleanup followed by silica cleanup.
10	Liquid/Liquid	Ethanol:Ethyl Acetate (5:95)	1 min with 20 g Na ₂ SO ₄ by high speed homogenizer		Gel permeation chromatography.
11	Soxhlet	Hexane:dithethyl ether (1:3)	8 hours	Sample ground with Na ₂ SO ₄ .	Silica-gel column chromatography (activated by 36 hours at 130C., 1.5g, column i.d.: 10mm.) after gel permeation chromatography (GPC) (Gel: Bio-bead S-X3, Column: 2cm i.d. 50cm length).
12	Liquid/Liquid with ultrasonication	Acetone/Cyclohexane	2 min + 1 min	Evaporation of lipid extract is done under stream of nitrogen.	Clean up with concentrated ultra clean sulfuric acid.
13	Hot Soxhlet	Hexane:Acetone (3:1; v/v)	2 hours	Samples mixed with Na ₂ SO ₄	Column chromatography on silica/acid silica elution with 15 ml hexane and 10 ml dichloromethane.
14	Liquid/Liquid	Pentane	15 min		Florisil SPE, sodium sulfate, extract with dichloromethane.
15	Pressurized Fluid Extraction (Dionex, ASE)	Dichloromethane	11 min	Preheat 0; Heat 5 min; Static 2 min; Flush 100 %; Purge 30 sec; Cycles 2; Pressure 1500 psi; Temp 100 °C; Cell size 22 ml	Pesticides: GPC. Florsil, Silsic acid (use 0.2 g equivalent of extract) PCB congeners; H4IIE procedure on the remainder of the extract.

Summary of Methods Used

Laboratory	Extraction Method	Extraction Solvent	Extraction Time	Extraction Other	Sample Extract Cleanup Method
16	Sample was mixed with about 50 g anhydrous sodium sulfate and extracted with mixed organic solvents.	petroleum ether/ether (1:1)	20 min		Silica gel cleanup. Two fractions eluted by hexane and benzene, respectively, were collected.
17	Chromaflex Column Extraction with sodium sulfate to grind & distribute sample.	Hexane, Methylene Chloride (1:1)	30 min		Automated gel permeation chromatography with hexane, methylene chloride (1:1). 8 grams of 100% activated Davisil 635 Type 60A silica gel in a 1 cm (ID) x 250 ml Chromaflex Column. Elution solvents 50 ml hexane, followed by 80 ml of hexane, methylene chloride (1:1).
18	Modified Folch method, at 1200 psi using an Accelerated Solvent Extractor (ASE)	2:1 (v/v) Chloroform:Methanol	2 cycles, approx. 20 min total		As per Christie, <u>Lipid Analysis</u> , 2003, pp101: 1/4 volume of 0.88% KCl is added to extract, then aqueous layer is removed, followed by second wash with 1/4 volume of 50% (aq) methanol, and removal of the aqueous layer. The lipid extract (in chloroform) is then reduced in volume to <1ml using a Rotovap.
19	Sample extraction: tissue was macerated with anhydrous sodium sulfate and extracted with hexane using sonication at room temperature.	hexane			Derivatization: fatty acid methyl esters (FAMEs) for SRM1945 were prepared using methanolic KOH at room temperature. (Christopherson, S. W. and Glass, R. L., 1969. Preparation of milk fat methyl esters by alcoholysis in an essentially nonalcoholic solution. J. Dairy Science 52, 1289-129.) FAMEs for QC05WB7 were prepared using 10% BF3 in methanol. Corresponding alcohols were not removed prior to instrumental analysis and likely affected quantitation of minor components following 16:1, 18:2 and the 24 carbon fatty acids.
20	Modified NOAA Status and Trends for Extraction of Biological Tissues for Trace Organics	dichloromethane:MEOH (3:1 v/v)- 0.01 % BHT added as preservative	10 min sonication		Florisil column used post derivatization. Picolinyl ester derivatization.
21	Accelerated solvent extraction (ASE)	Dichloromethane	~16 min	ASE conditions: Pressure = 2000 psi, temperature = 100 °C	

Summary of Methods Used

Laboratory		Instrument	Column Phase	Length (m)	Column i.d. (mm)	Film Thickness (μm)	Points	Conc. Range	Analytes Outside of Calibration Range
1	Pest.	GC-MS	DB-XLB	30	0.18	0.18	6	0.7 ng to 250 ng	none
	PCB	GC-MS	DB-XLB	30	0.18	0.18	6	0.7 ng to 250 ng	none
	PBDE	GC-MS	DB-XLB	30	0.18	0.18	6	0.7 ng to 250 ng	none
2	Pest.	GC/MS	HP-5MS	30	0.25	0.25	5	5 ng to 300 ng extracted	
	PCB	GC/MS	HP-5MS	30	0.25	0.25	5	5 ng to 300 ng extracted	
3	Pest.	GC/MS	DB-XLB	60	0.25	0.25	6	about 8 to 438 ng extracted	2,4'-DDT; 4,4'-DDT; 4,4'-DDE; 4,4'-DDD, trans-nonachlor PCBs 99, 101, 118, 138, 149, 153, 180, 187
4	PBDE								
	Pest.	GC/MS (SIM)	DB-5	60	0.25	0.25	5 to 10	0.003-100 ng/μL	PCBs 95, 99, 149, 151, 158, 183, 199 (in WB7 only)
5	PCB	GC/MS (SIM)	DB-5	60	0.25	0.25	5 to 8	0.003-10 ng/μL	
	Pest.	HPLC-PDA	2 (5-PYE) analytical columns in series	0.25	4.6	5 μm particles	1	0.322 ng/μL	
6	PCB	HPLC-PDA	2 (5-PYE) analytical columns in series	0.25	4.6	5 μm particles	1	0.322 ng/μL	
	Pest.	GC-MS SIM	DB-5	30	0.25	0.25	5	.2-1 -2 -5 -15 ng/ul	lower than 0.2 ng/ul: 2,4 DDE; 2,4 DDD; HCB; Hepachlor Epoxide, cis-Chlordane; trans-Chlordane; Oxychlordane; Mirex (SRMs)
	PCB	GC-MS SIM	DB-5	30	0.25	0.25	5	.2-1-2-5-9.25 ng/ul	lower than 0.2 ng/ul: PCBs 18; 44; 49; 52; 105; 151; 156; 170/190; 183; 194; 195; 206/209; 66; 95; 28/31; 87/115; 101/87/90; 106/118/123; 128/167; 45; 48; 74/61; 76/70; 92; 84; 119; 110; 82; 107/108; 154; 146; 141; 130; 159; 188; 184; 174; 177; 189; 202; 207(SRMs)
	PBDE	GC-MS SIM	DB-5	30	0.25	0.25	5	.2-.5-1-2-3 ng/ul	lower than 0.2 ng/ul: PBDEs 47; 99; 100; 153; 154; 28 (SRMs)

Summary of Methods Used									
Laboratory		Instrument	Column Phase	Length (m)	Column i.d. (mm)	Film Thickness (μm)	Points	Conc. Range	Analytes Outside of Calibration Range
7	Pest.	GC-ECD	DB-5	60	0.25	0.25	1	100 ng/ml	4,4'-DDE (All Homog VII & All SRM 1945 analyses); t-Nonachlor (Homog VI analysis 2 & 3) PCBs 138, 149, 153, & 180 (All Homog VII analyses); PCBs 118 & 187 (Homog VI analyses 2 & 3) See notes 3 and 4 at the end of this report.
	PCB	GC-ECD	DB-5	60	0.25	0.25	1	100 ng/ml	
	PBDE	GC-MS	DB-5	15	0.25	0.25	1	100-550 ng/ml	
8	Pest.	GC-MS-SIM	DB-5MS	30	0.25	0.25	4	5-200 ng/mL	
	PCB	GC-MS-SIM	DB-5MS	30	0.25	0.25	4	5-200 ng/mL	
	PBDE								
9	Pest.	GC-ECD	DB5	50	2	0.33	7	0.5-100 ng/ml	4,4'-DDE, 4,4'-DDT
	PCB	GC-ECD	DB5	50	2	0.33	7	0.5-100 ng/ml	153
	PBDE	GC-ECD	HP-5	30	0.25	0.25	4	0.6-120 pg/μL	
10	Pest.	GC-ECD	DB-608	30	0.53	0.83 μm	3	50-2000 ppb	Aldrin
	PCB						3	DDE & Dicofol)	p,p'-DDE,
11	PBDE	GC-EI-MSD	DB-1	30	0.25	0.25	8	4 - 1000 ng/ml	
12	Pest.	GC-ECD	SPB-5	60	0.25	0.25	5	0.48-104 ng/ml	The samples were diluted prior GC analysis to ensure that all compounds were within the range. The range varies from compound to compound.
	PCB	GC-ECD	SPB-5	60	0.25	0.25	5	0.59-91.2 ng/ml	
	PBDE	GC-NCI-MS	SPB-5	40	0.25	0.25	12	0.1-100 ng/ml	
13	Pest.								
	PCB	GC/MS (EI)	DB-1	30	0.25	0.25	7		none
	PBDE	GC/MS (ECNI)	HT-8	25	0.22	0.25	7		none
14	Pest.	GC/ECD	HP50+/HP5 MS	30/30	0.25/0.25	0.25/0.25		1,000 to 10 ppb 1000 to 10 ppb	none none
	PCB								
	PBDE								
15	Pest.	GC-ECD	DB-608	30	0.53	0.83	3	2 to 250 pg/μl	Dilute to inside of curve
	PCB	GC-ECD	DB-5	30	0.53	1.5	5	1 to 200 pg/μl	Dilute to inside of curve
	PBDE	GC-ECD	DB-XLB	60	0.25	0.25	4	0.5 to 500 pg	Dilute to inside of curve
16	Pest.	GC-ECD	DB608/DB1701	30/15	0.32/0.32	0.5/0.25	4 or 5	0.001-0.50 or 0.001-1.0	none
	PCB								
17	Pest.	GC/uECD	5% Phenyl Methylpolysiloxane	60	0.25	0.25	5	1-75 pg/μl	
	PCB	GC/uECD	5% Phenyl Methylpolysiloxane	60	0.25	0.25	5	1 - 100 pg/μl	
18	Fatty Acid								
19	Fatty Acid	GC-FID/MS	HP-225	30	0.25	0.25			
20	Fatty Acid	GC-MS	DB-5	30	0.25	0.25			
21	Fatty Acid	GC/MS (SIM)	DB-23	60	0.25	0.25	8	0.01-40 ng/μL (as methyl esters)	

Summary of Methods Used

Laboratory		Method of Quantitation	Added Prior to Extraction	Identity of Internal Standards Added Prior to Chromatographic Analysis
1	Pest.	IS	4,4'-DDD-D8, 4,4'-DDT-d8, 13C-cis chlordane	
	PCB	IS	¹³ C labeled PCBs 28, 52, 118, 153, 180, 194, 206, and 209	
	PBDE	IS	¹³ C BDE 99	
2	Pest.	IS	carbon-13 labeled lindane, trans-nonachlor, 4,4'-DDE, and 4,4'-DDT	
	PCB	IS	PCB 103 and PCB 198	
3	Pest.	IS		
	PCB	IS		
4	Pest.	IS	CB103	tetrachloro-o-xylene
	PCB	IS	CB103	tetrachloro-o-xylene
	PBDE	IS	CB 103	tetrachloro-o-xylene
5	Pest.	IS	1,2,3,4-tetrachloro-p-dibenzodioxin	1,7,8-trichloro-p-dibenzodioxin
	PCB	IS	1,2,3,4-tetrachloro-p-dibenzodioxin	1,7,8-trichloro-p-dibenzodioxin
6	Pest.	IS	4,4'-DDE13C12,HCB13C6,g-Chlordane13C10	Phenanthrene d12
	PCB	IS	BZ-3,15,28,52,118,153,180,194,208,209, all 13C12	Phenanthrene d12
	PBDE	IS	BDE100, BDE183, both 13C12	Phenanthrene d12
7	Pest.	IS	Ronnel	Tetrachloro-m-xylene (TCMX)
	PCB	IS	4,4' Dibromo octafluorobiphenyl (DOB) & PCB 198	PCB 103 & 3,3',4,4'-Tetrabromobiphenyl (TBB).
	PBDE	ES		
8	Pest.	IS	4,4'dibrooctafluorobiphenyl, PCB 103, PCB 198	Tetrachloro-meta-xylene
	PCB	IS	4,4'dibrooctafluorobiphenyl, PCB 103, PCB 198	Tetrachloro-meta-xylene
	PBDE			
9	Pest.	IS		PCB53
	PCB	IS		PCB53
10	Pest.	ES		
11	PBDE	IS		13C12-BDE-139
12	Pest.	IS	PCB 29, 112, 207	
	PCB	IS	PCB 29, 112, 207	
	PBDE	IS	BDE-119, 181	
13	PCB	IS	PCB 46, PCB 143	
	PBDE	IS	BDE 77, BDE 128	
14	Pest.	ES		
	PCB	ES		
15	Pest.	ES		
	PCB	ES		
	PBDE	ES		
16	Pest.	ES		
17	Pest.	IS	Octachloronaphthalene	
	PCB	IS	Octachloronaphthalene	
19	Fatty Acid	IS	C19:2n-6FAME	
20	Fatty Acid	IS	19:0 fame	
21	Fatty Acid	IS	C11:1 (as triglyceride)	C13:0 (as methyl ester)

Summary of Methods Used

Laboratory	Any Other Internal Standards?		Added When?	IS Surrogate Standards Used for Quantitation Were Added:	If the IS/surrogates Added After Extraction/Cleanup, Were Results Corrected for Recovery?
1				Prior to extraction	
2				Prior to extraction	
3				Prior to extraction	
4	Yes		Just before HPLC-SEC	Prior to extraction	
5				Prior to extraction	
6				Prior to extraction	
7	Pest. PCB	1,2,3-trichlorobenzene PCB 192		those added after extraction prior to chromatographic analysis	
8	Pest.			Prior to extraction	
11	Pest. PCB PBDE	(All 13 C12-PBDEs) BDE-3, BDE-15, BDE-28, BDE-47, BDE-99, BDE-153, BDE-154, BDE-183, BDE-197, BDE-207, BDE-209	Just prior to GPC	Prior to GPC	
12				Prior to extraction	
13				Prior to extraction	
21	Fatty Acid	C13:1 (as triglyceride)	Just prior to derivitization	those added after extraction/cleanup and just prior to chromatographic analysis (C13:1, as acid)	Yes

Summary of Methods Used

Laboratory	Recovery Range (%)	Were PCBs Separated From Pesticides Prior to GC?	Does PCB 132 coelute with PCB 153 or with PCB 105 or is it separated from both?
1		No	PCB 132 coelutes w/153
2		No	PCB 132 coelutes w/153
3		No	PCB 132 coelutes w/153
4	Pest. 106-111 PCB 106-111 PBDE 106-111	No	PCB 132 coelutes w/153
5	Pest. 83-94 PCB 83-94	No	
6		No	132/153/168 co-elute
7	Ronnel: Homog. VII (136 ± 8%), SRM1945 (145 ± 6%); 123-TCB: Homog. VII (93 ± 3%), SRM1945 (77 ± 3%) DOB: Homog. VII (114 ± 5%), SRM1945 (107 ± 5%); PCB 198: Homog. VII (121 ± 4%), SRM1945 (134 ± 8%); PCB 192: Homog. VII (98 ± 4%), SRM1945 (102 ± 2%) PCB See notes PBDE	No	See Notes
8		No	separates
9		Yes	
12		No	separates
13		No	separates
	PCB 75-90 PBDE 75-90		
14		No	
15		yes	separates
16		yes	
17		Yes	separates
21	Fatty Acids 92-99		

Appendix F

Additional analyte data and notes reported by individual laboratories.

Laboratory Additional Data and Notes

		Homog VII Sample 1 (ng/g wet wt) 2401	Homog VII Sample 2 (ng/g wet wt) 2599	Homog VII Sample 3 (ng/g wet wt) 2209	SRM 1945 Sample 1 (ng/g wet wt) 235	SRM 1945 Sample 2 (ng/g wet wt) 235	SRM 1945 Sample 3 (ng/g wet wt) 226
2	PCB 153/132						
3	PCB 45 PCB 70 PCB 74 PCB 82 PCB 92 PCB 107 PCB 110 PCB 146 PCB 154 PCB 157 PCB 158 PCB 163 PCB 174 PCB 193	Homog VII Sample 1 (ng/g wet wt) 4.35 5.13 121 30.8 118 10.1 43.4 377 26.6 27.5 77.1 272 211 57.0	Homog VII Sample 2 (ng/g wet wt) 4.03 4.60 122 30.4 117 9.7 43.2 374 26.4 28.4 78.0 268 209 56.5	Homog VII Sample 3 (ng/g wet wt) 4.27 5.10 117 28.8 112 20.8 41.8 364 26.3 27.4 75.6 263 208 56.8	SRM 1945 Sample 1 (ng/g wet wt) <2 11.29 19.2 5.92 20.8 4.58 37.7 50.2 3.69 3.49 9.39 47.0 26.70 10.1	SRM 1945 Sample 2 (ng/g wet wt) <2 13.06 21.5 6.54 23.3 4.83 41.0 53.6 4.22 4.03 9.45 49.1 28.55 10.4	SRM 1945 Sample 3 (ng/g wet wt) <2 11.54 19.4 6.27 20.9 4.67 39.6 48.8 3.42 3.44 8.88 47.8 26.04 9.60
4	Pesticide PCB Congeners	Homog VII Analysis A (ng/g wet wt) <1.7 <1.80 <2.18 <2.17 197	Homog VII Analysis B (ng/g wet wt) <1.80 <1.80 <1.70 201	Homog VII Analysis C (ng/g wet wt) <2.38 <2.39 <2.37 208	SRM 1945 Analysis A (ng/g wet wt) <1.70 <1.70 <1.70 20.4	SRM 1945 Analysis B (ng/g wet wt) 1.73 2.66 9.94	SRM 1945 Analysis C (ng/g wet wt) 17.0 1.70 17.0
	aldrin endosulfan I heptachlor nonachlor III 17 18 33 70 74 82 110 158 170 (separated from PCB 190) 171 177 191 205 208	Homog VII Sample 1 (ng/g wet wt) 1.32 3.12 <2.17 <2.17 103 12.9 38.5 75.6 282 72.6 194 8.93 5.12 42.3	Homog VII Sample 2 (ng/g wet wt) 1.15 3.33 <1.79 <1.80 104 12.9 38.9 75.2 286 72.7 200 9.08 5.40 43.2	Homog VII Sample 3 (ng/g wet wt) 0.914 3.32 <2.38 <2.38 104 13.2 39.4 76.1 299 74.9 9.67 <1.72 <1.71 43.4	SRM 1945 Sample 1 (ng/g wet wt) 1.73 2.66 <1.70 9.94 16.7 4.03 34.8 9.69 41.9 11.0 29.8 <1.72 <1.71 23.6	SRM 1945 Sample 2 (ng/g wet wt)	SRM 1945 Sample 3 (ng/g wet wt)
	Note: The analysis for PBDEs was performed on the same fraction as for pesticides/PCBs, using the same surrogate standard (PCB103). PBDE CONGENER ANALYSES	Homog VII Analyst (Initials) Date(s) of measurements (m/d/y)	Homog VII RHB 4/11/2005	Homog VII RHB 4/11/2005	Homog VII RHB 4/11/2005	SRM 1945 Sample 1 RHB 4/11/2005	SRM 1945 Sample 2 RHB 4/11/2005
	Congener PBDE 47 PBDE 99 PBDE 100 PBDE 153 PBDE 154 PBDE 28 PBDE 49 PBDE 66 PBDE 85 PBDE 183 Br6Unk#2 Br7Unk#1 Calibration Curve - PBDEs	Homog VII Sample 1 (ng/g wet wt) 147 24.7 37.1 14.7 35.7 3.86 4.34 3.74 <1.96 <1.98 24.1 2.42	Homog VII Sample 2 (ng/g wet wt) 156 26.5 41.3 15.4 38.2 4.06 4.80 4.33 <1.62 <1.64 34.3 2.64	Homog VII Sample 3 (ng/g wet wt) 157 27.8 40.7 16.0 38.5 4.20 4.80 4.34 <2.15 <2.17 25.9 2.55	SRM 1945 Sample 1 (ng/g wet wt) 37.0 15.4 8.44 7.46 11.3 1.75 2.44 <1.54 <1.54 1.59 4.31 <1.55	SRM 1945 Sample 2 (ng/g wet wt)	SRM 1945 Sample 3 (ng/g wet wt)
	PBDE Congeners	Points 5	Conc. Range 0.0025-2.5 ng/µL	Analytes outside of calibration curve calibration range none			

Additional Data and Notes (Continued)

5	Pesticide/PCB CONGENER ANALYSES					
	Homog VII Sample 1 DB	Homog VII Sample 2 DB	Homog VII Sample 3 DB	SRM 1945 Sample 1 DB	SRM 1945 Sample 2 DB	SRM 1945 Sample 3 DB
Analyst (Initials)						
Date(s) of measurements (m/d/y)	04/27/05	04/27/05	04/27/05	04/27/05	04/27/05	04/27/05
PCB Congener						
77	Homog VII (ng/g wet wt)	Homog VII (ng/g wet wt)	Homog VII (ng/g wet wt)	SRM 1945 (ng/g wet wt)	SRM 1945 (ng/g wet wt)	SRM 1945 (ng/g wet wt)
126	<1.3	<1.3	<1.1	<1.1	<1.1	<1.2
157	<1.1	<1.1	<1.0	<0.96	<0.99	<1.0
169	30.2	31.3	31.8	<0.70	<0.71	<0.74
170 + 194	<1.7	<1.7	<1.5	<1.4	<1.5	<1.5
189	431	441	446	93.9	95.7	94
	10.1	11.3	10.5	2.78	<0.72	<0.75
Sum PCBs	11400	11700	12100	1850	1870	1840
Sum DDTs	12950	12970	12960	941	917	922
LIPID CLASS ANALYSES						
Analyst (Initials)	Homog VII Sample 1 KT	Homog VII Sample 2 KT	Homog VII Sample 3 KT	SRM 1945 Sample 1 KT	SRM 1945 Sample 2 KT	SRM 1945 Sample 3 KT
Date(s) of measurements (m/d/y)	05/24/05	05/24/05	05/24/05	05/24/05	05/24/05	05/24/05
Wax esters	93.5	94.3	94.7	1.20	1.08	1.09
Triglycerides	6.54	5.66	5.28	98.8	98.9	98.9
Free fatty acids	0	0	0	0	0	0
Cholesterol	0	0	0	0	0	0
Phospholipids	0	0	0	0	0	0
6	PCB Congeners	Homog VII Sample 1	Homog VII Sample 2	Homog VII Sample 3	SRM 1945 Sample 1	SRM 1945 Sample 2
28/31	75.43	75.78	71.24	57.46	66.41	60.78
87/115	166.46	162.25	166.66	41.33	41.53	37.3
101/89/90	642.14	627.84	650.65	107.33	107.05	102.08
106/118/123	919.45	890.7	889.85	116.7	117.13	116.26
128/167	217.98	218.35	220.42	40.29	40.05	38.48
132/153/168	2885.03	2870.44	2929.8	363.45	362.71	352.98
138/163/158/164	2008.46	2001.22	2047.63	246.47	244.85	239.44
tetrapcb50	8.4	8.27	7.48	<1.33	<1.33	<1.33
tetrapcb45	13.4	13.43	13.11	10.51	10.66	8.99
tetrapcb48	75.4	75.68	74.73	26.07	26.05	24.29
tetrapcb74-61	139.58	136.42	134.46	48.58	47.99	42.81
tetrapcb76-70	44.41	41.57	37.92	43.21	42.23	36.88
tetrapcb81	13.49	13.59	12.58	<0.95	<0.95	<0.95
pentapcb92	93.96	92.46	94.48	29.13	28.53	26.46
pentapcb84	47.36	47.8	46.96	14.57	14.56	12.92
pentapcb119	26.41	26.01	25.2	15.05	15.07	12.8
pentapcb110	39.34	38.62	39.32	33.94	36.32	35.52
pentapcb82	15.49	15.22	15.05	8.65	8.74	7.76
pentapcb107-108	N/D	N/D	N/D	30.43	30.54	25.63
pentapcb 114	28.74	28.21	27.42	<1.86	<1.86	<1.86
hexapcb154	31.28	30.82	31.43	9.12	9.08	8.1
hexapcb146	329.49	325.36	337.03	37.19	36.85	38.8
hexapcb 141	127.31	125.37	127.57	24.44	26.45	25.08
hexapcb130	97.63	98.36	96.82	15.34	15.28	14.31
hexapcb159	24.39	25.03	24.23	8.78	8.74	7.8
hexapcb157	28.62	28.66	28.25	<0.81	<0.81	<0.81
heptapcb188	7.89	7.89	7.73	5.24	5.28	4.42
heptapcb 184	7.26	7.17	6.93	5.47	5.56	4.93
heptapcb174	191.99	201.28	209.8	27.58	28.82	29.04
heptapcb 177	160.4	169.72	177.88	29.8	28.73	28.82
heptapcb172	75.4	81.71	83.36	16.71	16.22	16.25
heptapcb 189	10.67	11.39	11.05	5.45	5.5	4.89
octapcb202	101.8	95.53	102.13	37.77	37.52	31.93
nonapcb 207	21.53	21.21	21.08	16.21	16.5	15.34
BDEs		6.67	6.01	5.73	5.39	4.98
bds28						4.72

Additional Data and Notes (Continued)

Additional Pesticides and PCBs	Homog VII Sample 1 (ng/g wet wt)	Homog VII Sample 2 (ng/g wet wt)	Homog VII Sample 3 (ng/g wet wt)	SRM 1945 Sample 1 (ng/g wet wt)	SRM 1945 Sample 2 (ng/g wet wt)	SRM 1945 Sample 3 (ng/g wet wt)
Heptachlor	1.11	DL	DL	DL	2.08	DL
Endrin	9.01	11.0	10.4	DL	DL	DL
Endosulfan I	Other ^E	Other ^E	Other ^E	Other ^E	Other ^E	Other ^E
Endosulfan II	6.35	7.25	6.18	44.8	45.0	45.8
Endosulfan Sulfate	30.3	24.7	19.0	148	147	146
BZ 8	Other ^B	Other ^B	Other ^B	Other ^B	Other ^B	Other ^B
BZ 77	Other ^G	Other ^G	Other ^G	Other ^G	Other ^G	Other ^G
BZ 110	Other ^G	Other ^G	Other ^G	Other ^G	Other ^G	Other ^G
BZ 126	5.07	5.26	4.69	23.5	24.8	24.8
BZ 169	Other ^D	Other ^D	Other ^D	Other ^D	Other ^D	Other ^D
Other: We found the following pairs of analytes coelute from our DB-5 column:						
OtherB : PCB 8 and alpha-HCH						
OtherD : PCB 169 and Mirex						

Additional Data and Notes (Continued)

7	<p>OtherE : PCB 101 and Endosulfan I</p> <p>OtherG : Since PCB 77 and PCB 110 coelute from our column and the response of each congener vary from each other, the relative ratios of two congeners can not be determined. We do not report the concentrations of either PCB 77 or PCB 110.</p>																																																																																				
Table 2: Recoveries of individual PBDE congeners spiked into dichlormethane																																																																																					
<table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>PBDE Congener</th> <th>Degree of Bromination</th> <th>Recovery (%)</th> </tr> </thead> <tbody> <tr><td>PBDE 3</td><td>1</td><td>86.7</td></tr> <tr><td>PBDE 7</td><td>2</td><td>84.9</td></tr> <tr><td>PBDE 15</td><td>2</td><td>98.4</td></tr> <tr><td>PBDE 17</td><td>3</td><td>98.5</td></tr> <tr><td>PBDE 28</td><td>3</td><td>98.9</td></tr> <tr><td>PBDE 49</td><td>4</td><td>108.6</td></tr> <tr><td>PBDE 71</td><td>4</td><td>101.0</td></tr> <tr><td>PBDE 47</td><td>4</td><td>105.1</td></tr> <tr><td>PBDE 66</td><td>4</td><td>103.6</td></tr> <tr><td>PBDE 77</td><td>4</td><td>107.6</td></tr> <tr><td>PBDE 119</td><td>5</td><td>107.8</td></tr> <tr><td>PBDE 99</td><td>5</td><td>111.2</td></tr> <tr><td>PBDE 100</td><td>5</td><td>105.6</td></tr> <tr><td>PBDE 85</td><td>5</td><td>101.8</td></tr> <tr><td>PBDE 126</td><td>5</td><td>104.4</td></tr> <tr><td>PBDE 154</td><td>6</td><td>97.5</td></tr> <tr><td>PBDE 153</td><td>6</td><td>96.9</td></tr> <tr><td>PBDE 138</td><td>6</td><td>92.8</td></tr> <tr><td>PBDE 156</td><td>6</td><td>82.7</td></tr> <tr><td>PBDE 184</td><td>7</td><td>87.3</td></tr> <tr><td>PBDE 183</td><td>7</td><td>80.6</td></tr> <tr><td>PBDE 191</td><td>7</td><td>66.1</td></tr> <tr><td>PBDE 197</td><td>8</td><td>59.3</td></tr> <tr><td>PBDE 196</td><td>8</td><td>43.0</td></tr> <tr><td>PBDE 207</td><td>9</td><td>46.7</td></tr> <tr><td>PBDE 206</td><td>9</td><td>17.8</td></tr> <tr><td>PBDE 209</td><td>10</td><td>11.5</td></tr> </tbody> </table>		PBDE Congener	Degree of Bromination	Recovery (%)	PBDE 3	1	86.7	PBDE 7	2	84.9	PBDE 15	2	98.4	PBDE 17	3	98.5	PBDE 28	3	98.9	PBDE 49	4	108.6	PBDE 71	4	101.0	PBDE 47	4	105.1	PBDE 66	4	103.6	PBDE 77	4	107.6	PBDE 119	5	107.8	PBDE 99	5	111.2	PBDE 100	5	105.6	PBDE 85	5	101.8	PBDE 126	5	104.4	PBDE 154	6	97.5	PBDE 153	6	96.9	PBDE 138	6	92.8	PBDE 156	6	82.7	PBDE 184	7	87.3	PBDE 183	7	80.6	PBDE 191	7	66.1	PBDE 197	8	59.3	PBDE 196	8	43.0	PBDE 207	9	46.7	PBDE 206	9	17.8	PBDE 209	10	11.5
PBDE Congener	Degree of Bromination	Recovery (%)																																																																																			
PBDE 3	1	86.7																																																																																			
PBDE 7	2	84.9																																																																																			
PBDE 15	2	98.4																																																																																			
PBDE 17	3	98.5																																																																																			
PBDE 28	3	98.9																																																																																			
PBDE 49	4	108.6																																																																																			
PBDE 71	4	101.0																																																																																			
PBDE 47	4	105.1																																																																																			
PBDE 66	4	103.6																																																																																			
PBDE 77	4	107.6																																																																																			
PBDE 119	5	107.8																																																																																			
PBDE 99	5	111.2																																																																																			
PBDE 100	5	105.6																																																																																			
PBDE 85	5	101.8																																																																																			
PBDE 126	5	104.4																																																																																			
PBDE 154	6	97.5																																																																																			
PBDE 153	6	96.9																																																																																			
PBDE 138	6	92.8																																																																																			
PBDE 156	6	82.7																																																																																			
PBDE 184	7	87.3																																																																																			
PBDE 183	7	80.6																																																																																			
PBDE 191	7	66.1																																																																																			
PBDE 197	8	59.3																																																																																			
PBDE 196	8	43.0																																																																																			
PBDE 207	9	46.7																																																																																			
PBDE 206	9	17.8																																																																																			
PBDE 209	10	11.5																																																																																			

Table 3: Concentrations of PBDE congeners with poor matching of mass spectral data.

Additional Polybrominated diphenyl ethers	Degree of Bromination	Homog VII Sample 1 (ng/g wet wt)	Homog VII Sample 2 (ng/g wet wt)	Homog VII Sample 3 (ng/g wet wt)	Homog VII Sample 1 (ng/g wet wt)	SRM 1945 Sample 2 (ng/g wet wt)	SRM 1945 Sample 3 (ng/g wet wt)
PBDE 3	1	12.3	10.8	10.1	12.3	19.2	14.4
PBDE 7	2	DL	DL	DL	DL	DL	DL
PBDE 15	2	DL	DL	DL	DL	DL	DL
PBDE 17	3	DL	DL	DL	DL	DL	DL
PBDE 28	3	4.50	DL	3.35	DL	DL	DL
PBDE 49	4	DL	DL	4.56	3.05	DL	3.09
PBDE 66	4	DL	DL	DL	DL	DL	DL
PBDE 71	4	DL	DL	DL	DL	DL	DL
PBDE 77	4	DL	DL	DL	DL	DL	DL
PBDE 85	5	DL	DL	DL	DL	DL	DL
PBDE 119	5	DL	DL	DL	DL	DL	DL
PBDE 126	5	DL	DL	DL	DL	DL	DL
PBDE 138	6	DL	DL	DL	DL	DL	DL
PBDE 156	6	DL	DL	DL	DL	DL	DL
PBDE 183	7	DL	DL	DL	19.9	DL	DL
PBDE 184	7	DL	DL	DL	DL	DL	DL
PBDE 191	7	DL	DL	DL	DL	DL	DL
PBDE 196	8	DL	DL	DL	DL	DL	DL
PBDE 197	8	DL	DL	DL	DL	DL	DL
PBDE 206	9	DL	DL	DL	DL	DL	DL
PBDE 207	9	DL	DL	DL	DL	DL	DL
PBDE 209	10	DL	DL	DL	DL	DL	DL

Addddtional Data and Notes (Continued)

11	HBCD ISOMER ANALYSES					
Analytical method used (e.g., GC-MS (include ionization type), GC-ECD):						
HBCD	Analyt. Instr.	Column Phase	Col. Length, m	Col. i.d., mm	particle size, μm	
HBCD-MS-MS C18 0.15 2.1 5 Agilent, ExtendC18						
Method of quantitation (IS = internal standard, ES = external standard):						
HBCD	IS					
If internal standard method was used, please complete the following section: Identity of internal standards/surrogates used that were added PRIOR to extraction of sample:						
HBCD	none					
Added after extraction/cleanup and JUST PRIOR to chromatographic analysis:						
HBCD	beta-HBCD-d18					
Any others? Added at what point in analyses: Added after extraction/ prior to GPC						
HBCD	C12-alpha-HBCD, 13C12-beta-HBCD, 13C12-gamma-HBCD					
IS/surrogate standards used for quantitation calculations were:						
X	those added prior to extraction those added after extraction/cleanup and just prior to chromatographic analysis those added after extraction/ prior to GPC					
If the IS/surrogates added after extraction/cleanup extraction were used for quantitation, were results corrected for percent recovery?						
Percent recovery range:						
Calibration Curve						
HBCD	Points 6	Conc. Range 0.4 - 400 ng/ml	Analytes outside of calibration curve calibration range			
			0.2 - 400 ng/ml			
RESULTS:						
Analyst (Initials)	Homog VII Sample 1 TI	Homog VII Sample 2 TI	Homog VII Sample 3 TI	SRM 1945 Sample 1 TI	SRM 1945 Sample 2 TI	SRM 1945 Sample 3 TI
Date(s) of measurements (m/d/y)	10/27/2005	10/27/2005	10/27/2005	10/27/2005	10/27/2005	10/27/2005
HBCD						
alpha-HBCD	Homog VII Analysis A (ng/g wet wt)	Homog VII Analysis B (ng/g wet wt)	Homog VII Analysis C (ng/g wet wt)	SRM 1945 Analysis A (ng/g wet wt)	SRM 1945 Analysis B (ng/g wet wt)	SRM 1945 Analysis C (ng/g wet wt)
beta-HBCD	15.1	18.0	17.2	8.1	7.2	NA
gamma-HBCD	<0.03	<0.03	<0.03	0.40	0.29	NA
	0.05	0.03	0.04	0.48	0.34	NA
12	TOXAPHENES					
Analyst (Initials)	Homog VII Sample 1 KIB/SIF/KBL	Homog VII Sample 2 KIB/SIF/KBL	Homog VII Sample 3 KIB/SIF/KBL	SRM 1945 Sample 1 KIB/SIF/KBL	SRM 1945 Sample 2 KIB/SIF/KBL	SRM 1945 Sample 3 KIB/SIF/KBL
Date(s) of measurements (m/d/y)	06.30.05	06.30.05	06.30.05	06.30.05	06.30.05	06.30.05
CHB-26	261.5	334.3	223.0	n.a	39.1	44.6
CHB-40	85.7	96.3	80.9	n.a	16.4	16.7
CHB-41	39.7	45.4	37.3	n.a	10.4	11.1
CHB-44	90.1	107.1	66.6	n.a	30.0	31.7
CHB-50	194.7	225.0	171.0	n.a	93.4	91.8
CHB-62	66.1	76.5	58.3	n.a	44.1	51.1
13	PCB CONGENER ANALYSES					
Congener	Homog VII Sample 1 (ng/g wet wt)	Homog VII Sample 2 (ng/g wet wt)	Homog VII Sample 3 (ng/g wet wt)	SRM 1945 Sample 1 (ng/g wet wt)	SRM 1945 Sample 2 (ng/g wet wt)	SRM 1945 Sample 3 (ng/g wet wt)
74	120.5	112.3	109.3	14.7	16	15
110	20.1	21.5	21	21.4	21.4	21.5
196	121.5	128.5	124.7	49.6	51.3	50.8
199	148.1	158.7	153.8	48.9	50.8	49.8
PBDE CONGENER ANALYSES						
Congener	Homog VII Sample 1 (ng/g wet wt)	Homog VII Sample 2 (ng/g wet wt)	Homog VII Sample 3 (ng/g wet wt)	SRM 1945 Sample 1 (ng/g wet wt)	SRM 1945 Sample 2 (ng/g wet wt)	SRM 1945 Sample 3 (ng/g wet wt)
28	2.02	1.83	1.97	1.15	1.11	1.09
49	2.12	1.79	1.99	1.16	0.97	1.06
66	3.76	3.56	3.63	1.39	1.24	1.29
85	2.22	1.56	3.29	NA	NA	NA
2'-MeO-BDE68	59.1	59.9	59.4	39.9	37.5	36.1
6-MeO-BDE47	500.1	467.8	457.7	49	48.9	47.1

Additional Data and Notes (Continued)

18	Fatty Acids	Homog VII Sample 1 (ng/g wet wt)	Homog VII Sample 2 (ng/g wet wt)	Homog VII Sample 3 (ng/g wet wt)	SRM 1945 Sample 1 (ng/g wet wt)	SRM 1945 Sample 2 (ng/g wet wt)	SRM 1945 Sample 3 (ng/g wet wt)
iso + antiso C5:0	< 0.01	< 0.01	< 0.01	< 0.01	< 0.01	< 0.01	< 0.01
4,8,12-trimethyltridecanoic acid (TMTD)	0.02	0.02	0.02	0.08	0.07	0.08	
(Z)-9-tetradecenoic acid (14:1n-5)	0.16	0.15	0.15	0.41	0.38	0.38	
iso 15:0	0.04	0.04	0.03	0.21	0.2	0.2	
antiso 15:0	0.03	0.03	0.02	0.08	0.08	0.08	
(Z)-7-hexadecenoic acid (16:1n-9)	0.41	0.41	0.42	1.99	1.976	1.88	
(Z,Z)-6,9-Hexadecadienoic acid (16:2n-7)	< 0.01	< 0.01	< 0.01	0.02	0.02	0.02	
(Z,Z)-9,12-Hexadecadienoic acid (16:2n-4)	0.06	0.07	0.11	< 0.01	< 0.01	< 0.01	
Iso17	0.03	0.03	0.04	0.12	0.11	0.11	
antiso17:0	< 0.01	0.01	0.01	0.07	0.07	0.07	
7-methyl-7-hexadecenoic acid (7M7H)	0.23	0.22	0.27	0.39	0.37	0.37	
phytanate	< 0.01	< 0.01	< 0.01	< 0.01	< 0.01	< 0.01	
(Z)-9-heptadecenoic acid (17:1n-8)	0.16	0.17	0.18	0.41	0.4	0.39	
(Z)-7-octadecenoic acid (18:1n-11)	2.1	1.97	1.93	2.7	2.7	2.5	
(Z)-13-octadecenoic acid (18:1n-5)	0.11	0.1	0.11	0.24	0.23	0.23	
(Z,Z)-11,14-Octadecadienoic acid (18:2n-4)	0.02	< 0.01	0.02	0.03	0.03	0.03	
(Z,Z,Z)-8,11,14-Eicosatrienoic acid (20:3n-6)	0.02	0.02	0.02	< 0.01	< 0.01	< 0.01	
(Z,Z,Z,Z)-8,11,14,17-Eicosatetraenoic acid (20:4n-3)	0.14	0.14	0.14	0.23	0.22	0.21	
Total reported	46.6	46.3	45.3	63.2	62.1	59.6	

19	Fatty Acids	Homog VII Sample 1 (ng/g wet wt)	Homog VII Sample 2 (ng/g wet wt)	Homog VII Sample 3 (ng/g wet wt)	SRM 1945 Sample 1 (ng/g wet wt)	SRM 1945 Sample 2 (ng/g wet wt)	SRM 1945 Sample 3 (ng/g wet wt)
iso 5:0					0.99	1.01	1.08
Iso 12:0					0.12	0.01	0.01
12:1n5					0.34	0.03	0.03
3-Me 13:0					1.00	0.10	0.11
13:1 n7					0.26	0.04	0.02
iso 13:0					0.10	0.01	0.01
anteiso 13:0					0.07	0.01	0.01
13:0	0.02	0.01	0.02	0.19	0.02	0.02	
iso 14:0	0.01	0.01	0.01	0.27	0.02	0.02	
14:1 n10	0.02	0.01	0.01	0.68	0.05	0.05	
14:1n7	0.03	0.05	0.06	0.76	0.07	0.06	
14:1n5	0.10	0.11	0.13	3.03	0.27	0.27	
14:0	1.19	1.33	1.41	27.33	2.81	2.60	
9-me 15:0	0.02	0.02	0.02	0.68	0.08	0.06	
iso 15:0	0.00	0.03	0.03	1.47	0.13	0.13	
anteiso 15:	0.02	0.02	0.02	0.70	0.06	0.06	
15:1n6				0.14	0.01	0.02	
12-me 16:0				0.07	0.01	0.01	
iso 16:0	0.05	0.07	0.06	1.20	0.19	0.12	
16:1n9	0.21	0.27	0.28	11.25	0.95	1.13	
16:1n5	0.03	0.05	0.05	0.71	0.06	0.07	
2,6,10,14-tetra methyl 19:0	0.02	0.02	0.02	0.52	0.07	0.06	
12-me 17	0.01	0.02	0.02	0.56	0.07	0.06	
17:1n9	0.18	0.19	0.21	2.79	0.29	0.25	
13 me 17:0				0.09	0.01	0.01	
iso 17:0	0.02	0.02	0.02	0.91	0.09	0.08	
anteiso 17	0.02	0.02	0.02	0.61	0.05	0.06	
17:1n8	0.12	0.13	0.13	2.52	0.26	0.21	
3,7,11,15-tetra methyl 20:0	0.01	0.02	0.02	0.76	0.07	0.07	
14-me 18:0				1.41	0.09	0.11	
18:1n11	1.80	3.22	3.27	36.90	3.57	3.07	
18:1n5	0.22	0.11	0.13	2.22	0.28	0.17	
20:4n3	0.07	0.07	0.07	0.47	0.10	0.09	
21:1n12	0.02	0.02	0.02				
21:1n10	0.02	0.02	0.02				
22:5n6				0.19	0.02	0.00	
22:2n9				0.34	0.04	0.03	
22:1n7	0.00	0.01	0.10				
22:0				0.22	0.04	0.03	
24:5n3				0.27	0.01	0.02	
24:1n11	0.03	0.01	0.01	0.33	0.02	0.02	

Additional Data and Notes (Continued)

20	Fatty Acid (as methyl ester)	Homog VII Sample 1 (%, wet weight)	Homog VII Sample 2 (%, wet weight)	Homog VII Sample 3 (%, wet weight)	SRM 1945 Sample 1 (%, wet weight)
Capric acid (C10:0)	<0.00491	<0.00495	<0.00499	0.0284	
C11:0	<0.00245	<0.00247	<0.00249	0.00461	
C12:1	<0.00491	<0.00495	<0.00499	0.00465	
isoC14:0	0.0161	0.0162	0.0167	0.0479	
C14:1n9*	0.0353	0.0367	0.037	0.102	
4,8,12-trimethyl C13:0*	0.00524	0.00601	0.00552	0.0274	
C14:1n7*	0.0549	0.0554	0.0563	0.133	
11-methyl C14:0*	0.00289	0.00295	0.00288	0.00596	
isoC15:0*	0.0417	0.0425	0.0413	0.228	
anteisoC15:0	0.0192	0.0197	0.0193	0.0665	
C15:1n5	<0.00245	0.0028	<0.00249	0.00365	
isoC16:0	0.0220	0.0229	0.0224	0.0890	
anteisoC16:0*	<0.00233	<0.00235	<0.00237	0.00525	
2,6,10,14-tetramethyl C15:0*	0.0321	0.0326	0.0304	0.0692	
C16:1n11*	0.103	0.107	0.106	0.195	
C16:1n9*	0.428	0.437	0.442	2.06	
C16:1n5*	0.0742	0.0756	0.075	0.204	
7-methyl C16:1*	0.0476	0.0493	0.0471	0.0648	
isoC17:0	0.0494	0.0504	0.0487	0.148	
C16:2n6*	0.023	0.0228	0.0233	0.320	
anteisoC17:0*	0.0171	0.0178	0.0171	0.0709	
C16:2n4*	0.102	0.105	0.104	0.173	
C16:3n6*	0.0156	0.0162	0.0133	0.0237	
C16:3n4*	0.0306	0.0290	0.0274	0.0331	
Margoleic acid (C17:1n?)*	0.260	0.262	0.264	0.405	
C17:1n7	0.00502	0.00705	0.00500	0.0105	
C16:4n3*	0.0352	0.0386	0.0348	0.192	
isoC18:0	0.0249	0.021	0.0205	0.0337	
anteisoC18:0*	0.00247	0.00222	<0.00204	0.00593	
C16:4n4*	0.0255	0.0246	0.0288	0.0331	
C18:1n13*	0.0217	0.0264	0.0255	0.0432	
C18:1n11*	2.05	2.05	2.04	2.67	
C18:1n5*	0.132	0.13	0.124	0.271	
C18:2n7*	0.0333	0.0334	0.034	0.0405	
C18:2n4*	0.0488	0.0491	0.0479	0.0641	
C19:0	0.0483	0.049	0.0471	0.0498	
C18:3n4*	0.0668	0.0694	0.0603	0.0371	
C18:3n1*	<0.00981	<0.00900	<0.00997	<0.00814	
C18:4n1*	0.0199	<0.0148	<0.0150	<0.0122	
C20:1n15	0.0264	0.0296	0.0250	0.0192	
C20:1n18	5.69	5.76	5.60	3.25	
C20:1n5*	0.0589	0.0598	0.0578	0.0514	
C20:2n9*	0.0251	0.0270	0.0241	0.00689	
dihomo-g-Linolenic acid (C20:3n6)	0.0514	0.0602	0.0515	0.0552	
C20:4n3*	0.173	0.181	0.174	0.228	
Behenic acid (C22:0)	0.0272	0.0279	0.0269	0.0331	
C22:1n7*	0.137	0.146	0.134	0.119	
C22:1n5*	<0.00981	<0.00900	<0.00997	<0.00814	
C22:5n3	0.0470	0.0575	0.0485	0.103	
C22:4n6	0.0564	0.0585	0.0500	0.103	
C22:3n3	<0.0160	<0.0161	<0.0163	<0.0133	
C22:4n3*	<0.0313	<0.0316	<0.0318	0.0470	
C22:1n11*					

§ C22:1n11 is quantitated using C:22:1n12 in calibration standards.

* Compounds are tentatively identified as to specific positional isomer, and are quantitated using response factor of closest retention time compound of similar structure; results should be considered semi-quantitative.